

Notice number: 6.001

COMMISSION OF INQUIRY INTO DNA PROJECT 13

Section 5(1)(d) of the *Commissions of Inquiry Act 1950*

STATEMENT OF GENEROSA LUNDIE

I, **Generosa Lundie**, care of Queensland Health Forensic and Scientific Service, Forensic Scientist, do solemnly and sincerely declare that:

1. On 19 October 2023, I was requested to provide a statement responding to Notice 6.001 "Requirement to Give Information in a Written Statement".

Identification

Question 1(a) - State your full name:

2. My full name is Generosa Lundie.

Question 1(b) - State your qualifications, skills or experience relevant to forensic science and DNA:

3. I graduated from Perpetual Help College of Medicine in the Philippines with a Bachelor of Science – Medical Technology in 1991.
4. I graduated from Griffith University with a Bachelor of Biomedical Sciences in 2005.
5. **Annexed and marked Exhibit GL-01** is a copy of my CV.

Question 1(c) - State the period(s) of time you have been or were employed by or otherwise engaged with Queensland Health, Queensland Health Forensic and Scientific Services (QHFSS) and/or Forensic Science Queensland, and in what roles and when.

6. I commenced working as a Laboratory Assistant at Queensland Health Forensic and Scientific Services – DNA Analysis between March and June 2006. This is now known as Forensic Science Queensland. Since then, I have been engaged in various roles with QHFSS and/or Forensic Science Queensland as set out below.

Automation Project Team – June 2006 to late-2008

7. Between approximately June 2006 to the end of 2008, I worked in the Automation Project Team as a newly graduated scientist and I was supervised by Thomas Nurthen who was the Project Manager for the team.
8. The members of the Automation Project Team were:
 - (a) Thomas Nurthen;
 - (b) Cecilia Iannuzzi;
 - (c) Iman Muharam;

Generosa Lundie

Witness

- (d) Vojtech Hlinka; and
 - (e) Breanna Gallagher.
9. Breanna and I were junior members of the team. The more senior scientists in the team were Thomas, Cecilia, Iman and Vojtech.
 10. While in the Automation Project Team, my duties as a newly graduated scientist involved:
 - (a) being trained in manual DNA extraction by Cecilia (Breanna was also trained at the same time with me);
 - (b) assisting in the preparation of mock samples to be used in the Project 9 and Project 11 discussed below;
 - (c) undertaking manual DNA extraction; and
 - (d) undertaking other tasks as instructed by Tom who was as the Project Manager of the Automation Project Team and the more senior scientists, being Cecilia, Iman and Vojtech.
 11. I understood the purpose of the Automation Project Team was to explore opportunities to use automation in the DNA extraction process. I recall there was a plan to incorporate an automated robotic platform so that both new manual and automated DNA extraction methods could be introduced.

Project 9

12. In the early part of my time in the Automation Project Team, I recall assisting the senior scientists (Cecilia, Iman and Vojtech) and Breanna with Project 9.
13. At the time I joined the Automation Project Team, the wider Forensic Team was using a DNA extraction solution called Chelex. At the time, if I recall correctly, there was a plan to stop using Chelex as a liquid agent to extract DNA because it took longer to process and apparently it could be harmful to scientists.
14. A DNA extraction kit is a small box that contains liquid agent solutions necessary for the DNA extraction process.
15. Based on my recent review of the Project 9 report, I believe Project 9 involved the evaluation of various commercial DNA extraction kits, which included:
 - (a) trialling six DNA extraction kits (including Chelex, DNA IQ and four others), using mock samples to identify which performed best; and
 - (b) performing manual DNA extraction processes with the different DNA extraction kits.
16. DNA IQ was one of the five new extraction kits that was trialled.
17. Based on my recent review of the Project 9 report, I believe that the related purpose of Project 9 was to identify the best extraction kits that could also be used or trialled in an

.....
 Generosa Lundie

.....
 Witness

automated procedure using an automated robotic platform, being the Multiprobe II platform. The Multiprobe II platform is a robot that automated the DNA extraction process. When I joined the Automation Project Team, there was one or two Multiprobe II platforms being trialled as part of Automation Project Team's work, but I was not involved in that work.

18. My involvement in Project 9 occurred a long time ago now, and I only remember bits and pieces such as assisting in the preparation of mock samples and performing laboratory work. I was not trained at that time in DNA analytical processes other than manual extraction. I was not involved in any analysis, evaluation or interpretation of results as I was still new and had limited experience in Forensics.
19. I am aware a report was prepared about Project 9.
20. I was not involved in interpreting the results or writing the report. I do not know who wrote the Project 9 report. My name is on page 1 of the Project 9 report along with all other members of the Automation Project Team and Vanessa Ientile. I believe all members of the team were named on the report to recognise we all made some wider contribution and to recognise the collective assistance with the work which supported the project.
21. **Annexed and marked Exhibit GL-02** is the Project 9 report I found on our digital storage system.

Project 11

22. I recall assisting Breanna and the senior scientists with Project 11.
23. Based on my recent review of the Project 11 report, I believe this project was about validating that DNA IQ kit (which was identified through Project 9) was the best to use when extracting DNA manually. Again, this took place a long time ago, and I can only recall bits and pieces. I was not involved in any analysis of the results. I assisted in laboratory duties as instructed by the senior scientists.
24. I am aware a report was prepared about Project 11. I may have had a brief look at the report before it was finalised, but I do not have a deep knowledge of the data presented in it. As mentioned, I was new to the team with limited experience in Forensics. I do not know who wrote the Project 11 report. I did not have any involvement in drafting the Project 11 report. I believe my name appears on the report to recognise all members of the Project Automation Team made some contribution to the work which supported the project.
25. **Annexed and marked Exhibit GL-03** is the Project 11 report I found on our digital storage system.
26. As a career development task, I asked Tom if I could attend the Australian and New Zealand Forensic and Scientific Services Symposium in 2008. I asked Tom if I could develop a poster about the outcome of Project 11 for the symposium. Tom agreed, and the poster I developed was approved by Tom and Iman. I displayed the poster at the symposium. After the symposium, the poster was made available to Forensic and Scientific Services staff to inform them about what was presented at the symposium.

.....


Generosa Lundie

.....


Witness

Annexed and marked Exhibit GL-04 is a copy of this poster I found on our digital storage system.

Project 13

27. I am aware there was a Project 13. I do not recall being involved with this project because between 2006 and 2008 if I recall correctly, I was heavily involved in manual DNA extraction processes. I think Project 13 occurred after Projects 9 and 11 were completed, but some work may have occurred simultaneously.
28. I do not recall reviewing or reading any version of the Project 13 report until I was provided with a copy in relation to this Inquiry. I do not know who wrote the Project 13 report. I did not have any involvement in drafting the Project 13 report. I believe my name appears on the report to recognise all members of the Project Automation Team made some contribution to the work which supported the project.
29. When I heard in early October 2023 that the Project 13 report was going to be the subject of this Commission of Inquiry, I looked at the report briefly, I did not read it in detail. I saw on pages 8 and 9 that there were highlighted sections and question marks, and this indicated to me that I was looking at a draft report.
30. **Annexed and marked Exhibit GL-05** is the Project 13 report I looked at for this purpose, with my markings.

Analytical Team – Late-2008 to August 2023

31. I think in late-2008 or early 2009, the Project Automation Team work finished and I was moved to the Analytical Team, where I remained until August 2023.
32. I reported to Allan McNeven and my work involved:
 - (a) General laboratory duties;
 - (b) Automated DNA extraction tasks;
 - (c) Manual DNA extraction tasks;
 - (d) Pre-PCR tasks;
 - (e) Capillary Electrophoresis tasks; and
 - (f) Non-laboratory tasks.

Evidence Recovery Team – August 2023 to present

33. In August 2023, I moved to the Evidence Recovery Team. The work in this team involves examination of items, examination of sexual assault kits currently called (FMEKs) and performing presumptive testing on samples under supervision before they are sent to the Analytical section for further testing.

Manual and Automated DNA Extraction Methods

Question 2 – In relation to the report being the “Project 13. Report on the Verification of an Automated DNA IO Protocol using the Multiprobe ILPLUS HT EX with Gripper

 Generosa Lundie

 Witness

Integration Platform”, Nurthen, T., Hlinka, V., Muharam, I., Gallagher, B., Lundie, G., Iannuzzi, C., Ientile, V. Automation/LIMS Implementation Project, DNA Analysis FSS (August 2008) (2008 Report)1 and the abstract and introduction therein which state:

1. Abstract

A manual method for extracting DNA from forensic samples using the DNA IQ™ system (Promega Corp., Madison, WI, USA) was validated for routine use in DNA Analysis (FSS). We have verified an automated DNA IQ™ protocol in 96-well format for use on the MultiPROBE® II PLUS HT EX Forensic Workstation platforms (PerkinElmer, Downers Grove, IL, USA). Data indicate that results from the automated procedure are comparable to those from the manual procedure. Contamination checks were performed using samples prepared in checkerboard and zebra-stripe format, and results were as expected. We recommend the use of the MultiPROBE® II PLUS HT EX platforms to perform automated DNA extraction using the DNA IQ™ system.

2. Introduction

The MultiPROBE® II PLUS HT EX FORENSIC WORKSTATION platforms (PerkinElmer, Downers Grove, IL, USA) are equipped to perform automated DNA extractions, as they include a DPC shaker and individual heat controllers to enable on-board lysis and incubation steps. Currently in DNA Analysis, the MultiPROBE® platforms allow walk-away operation of PCR setup protocols for DNA quantitation and amplification.

The DNA IQ™ protocol has been verified or validated by various laboratories for use on the MultiPROBE® II PLUS platform. The laboratories that perform an automated DNA IQ™ protocol include PathWest (Western Australia), Forensic Science South Australia (South Australia) and Centre of Forensic Sciences in Toronto (Ontario). The MultiPROBE® II PLUS instrument comes pre-loaded with an automated DNA IQ™ protocol. Unlike the other laboratories, however, we did not validate the included protocol, but instead validated a manual DNA IQ™ protocol which was based on the CFS automated protocol (PerkinElmer, 2004), followed by verification of an automated protocol based on the validated manual method.

The verified automated DNA IQ™ protocol is identical to the validated manual protocol used in-house: there are no differences in reagents or volumes. The adopted DNA IQ™ protocol differs slightly, however, from the manufacturer's protocol, as it includes a lysis step using Extraction Buffer (10mM Tris, 1mM EDTA, 100mM NaCl, 20% w/v SDS) in the presence of Proteinase K, before incubating in the DNA IQ™ Lysis Buffer. Furthermore, the lysis incubation conditions were lowered from 70°C to 37°C in order to accommodate extraction of DNA from heat labile materials such as nylon and polyester. In addition, the automated protocol utilises the SlicPrep™ 96 Device (Promega Corp., Madison, WI, USA) for simultaneous processing of samples in a 96-well format.

Manual Method

Question 2(a) describe, with precision, the “manual method” for extracting DNA from forensic samples using the DNA IQ™ system referred to in the first line of the Abstract to the 2008 Report (Manual Method), including whether the Manual Method:

- (i) **was devised within the QFSS Forensic DNA Analysis laboratory (Laboratory); or**
 - (ii) **was otherwise a modification of an existing manual method (and if so which method),**
34. The DNA IQ system came in a kit or box containing different chemical liquid solutions used for extracting DNA. I am not able to describe the method with precision without referring to the manual extraction instructions outlined in the relevant written standard operating procedure which we followed at the time. It has been at least 10 years since I performed the procedure for manual extraction using DNA IQ. I can only remember bit and pieces.
35. As I recall, the manual method for extracting DNA using DNA IQ involved the following steps:
- (a) Step 1 – A scientist would receive from the Evidence Recovery Team a tube containing a piece of substrate (which might be a piece of cotton or fabric collected by police from a crime scene) which might contain a DNA sample. The scientist would add a volume of solution 1 (called the extraction buffer) using a

.....
Generosa Lundie

.....
Witness

pipette. The scientist would then incubate the tube to heat the solution which opens the cell membrane.

- (b) Step 2 – The scientist would then remove the tube from incubation and add solution 2 (which is a lysis buffer) and solution 3 (which is a resin containing paramagnetic beads). These solutions were mixed to break down the cells and isolate the DNA. After mixing, the scientist would remove all liquid from the tube using a pipette so the DNA is left attached to the paramagnetic resin beads.
 - (c) Step 3 – The scientist would then add a volume of solution 4 (which is called the wash buffer) to the tube and mixed it. The scientist then removed all liquid from the tube using a pipette. The DNA which had bound to the resin would remain in the tube. This washing process would be repeated three times so all remaining contaminants or impurities from the DNA were removed and ideally only pure DNA would remain.
 - (d) Step 4 – The tube containing the DNA was then opened and left to dry inside a extraction cabinet fume hood for a period of time to remove inhibitors such as alcohol.
 - (e) Step 5 – The scientist would then add solution 5 (which is an elution buffer) to the tube to release DNA from the paramagnetic resin beads. The scientist collected the solution containing the DNA using a pipette and transferred it to another tube. The scientist repeated this process (i.e. solution 5 was added again, and the DNA was collected again). The tube containing the extracted DNA was stored and was then ready for the next stages of processing.
36. After the manual extraction process was complete, another member of the Analytical Team would perform the next stages of processing being:
- (i) DNA quantification.
 - (ii) DNA amplification; and
 - (iii) Capillary electrophoresis,
- to produce a DNA profile result which would then be reviewed by the case scientist for DNA comparison.
37. I do not know where this manual method was devised.
38. I do not know whether it modified an existing manual method.
39. I was trained in the manual extraction process by Cecilia between 2006 and 2007 when I commenced in the Automation Project Team. This training involved me:
- (a) observing Cecilia performing the manual extraction process three times;
 - (b) performing the manual extraction process three times under Celia's supervision;
 - (c) discussing my competence with Cecilia;

.....


Generosa Lundie

.....


Witness

- (d) completing a training module, answering both oral and written questions within module;
- (e) being signed-off by Cecilia as competent to perform manual extraction procedure using DNA IQ.

Question 2(b) describe, with precision, the method by which the Manual Method’s “routine use” in DNA Analysis (FSS) was validated

40. Based on my recent review of the Project 11 report, I understand that Project 11 involved validation of the use of DNA IQ, but my involvement in that project as I recall was limited to performing laboratory duties which was manual extraction processes only.
41. I was not involved in the overall validation or the collection and assessment of the outcome of results.

Question 2(c) state whether, and if so how, the Manual Method differed from or otherwise modified the DNA IQ™ protocol that was “verified or validated by various laboratories for use on the Multiprobe® II PLUS platform” (as stated in the second line of the second paragraph of the Introduction to the 2008 Report)

42. I do not know the answer to this question. I do not recall being specifically involved in any modified version of using DNA IQ nor do I recall being involved in any verification of the Multiprobe® II PLUS platform.

Question 2(d) state when the Manual Method was so devised

43. I do not know when the manual method was devised. I was only instructed to undertake manual DNA extractions to assist my team members.

Question 2(e) identify those within the Laboratory responsible for devising the Manual Method

44. I do not know who was responsible for devising the manual method.

Question 2(f) state the reason(s) why the Laboratory chose to devise and to implement the Manual Method

45. I do not know.

CFS Automated Protocol

Question 2(g) describe, with precision, the “CFS automated protocol (PerkinElmer, 2004)” (CFS Automated Protocol) referred to in the seventh line of the second paragraph of the Introduction to the 2008 Report

46. I do not know what this is referring to.

Manual DNA IO™ Protocol

Question 2(h) describe, with precision, the “manual DNA IQ™ protocol” (Manual DNA IQ™ Protocol)” referred to in the seventh line of the second paragraph of the Introduction to the 2008 Report, including whether it: [REDACTED]

.....
Generosa Fundie Witness

- (i) was developed or otherwise supplied by the manufacturer of the **MultiPROBE® II PLUS HT EX FORENSIC WORKSTATION** platform;
- (ii) was devised within the Laboratory; or
- (iii) was otherwise a modification of an existing **Manual DNA IQ™** protocol (and if so which method)

47. See above at paragraphs [35] to [39].

Question 2(i) describe, with precision, the method by which the Manual DNA IQ™ Protocol was validated

48. I do not know how the manual method using DNA IQ was validated.

Question 2(j) state whether, and if so how, the Manual DNA IQ™ Protocol differed from or otherwise modified the DNA IQ™ protocol that was “verified or validated by various laboratories for use on the Multiprobe® II PLUS platform” (as stated in the second line of the second paragraph of the Introduction to the 2008 Report)

49. I do not know.

Question 2(k) state when the Manual DNA IQ™ Protocol was so devised

50. I do not know when the manual method using DNA IQ was devised.

Question 2(l) identify those within the Laboratory responsible for devising the Manual DNA IQ™ Protocol

51. I do not know.

Question 2(m) state the reason(s) why the Laboratory chose to devise Manual DNA IQ™ Protocol

52. I do not know.

Automated DNA IQ™ Protocol

Question 2(n) state whether the “automated DNA IQ™ protocol” referred to in the first line of the third paragraph of the Introduction to the 2008 Report (Automated DNA IQ™ Protocol) is the same as the automated protocol the subject of the 2008 Report. If it is not, then state the reasons why and describe any differences

53. I do not know.

Question 2(o) state whether, and if so how, the Automated DNA IQ™ Protocol differed from or otherwise modified:

- (i) the Manual Method;

.....

 Generosa Lunde

.....

 Witness

- (ii) the DNA IQ™ protocol that was “verified or validated by various laboratories for use on the Multiprobe® II PLUS platform” (as stated in the second line of the second paragraph of the Introduction to the 2008 Report);
- (iii) the CFS Automated Protocol; and
- (iv) the Manual DNA IQ™ Protocol

54. I do not know.

Question 2(p) state when the Automated DNA IQ™ Protocol was so devised

55. I do not know.

Question 2(q) identify those within the Laboratory responsible for devising the Automated DNA IQ™ Protocol

56. I do not know.

Question 2(r) state the reason(s) why the Laboratory chose to devise the Automated DNA IQ™ Protocol rather than use the manufacturer method

57. I do not know.

Multiprobe II PLUS HT EX with Gripper Integration Platform (Multiprobe II Device)

Question 3 - State when the Laboratory received the Multiprobe II Device

58. I do not know when the laboratory received the Multiprobe II Device.

59. The Multiprobe II Device if I recall correctly was in the laboratory when I commenced in June 2006.

Question 4 - For each of the Manual DNA IQ™ Protocol and the Automated DNA IQ™ Protocol, describe, with precision and completeness, what, if anything was done to the device to modify it, including whether any of the manufacturer's factory settings were changed, and if so which ones and how (including but not limited to temperature settings, reagents and volumes)

60. I do not know. Again, my task was very specific and limited to just assisting in laboratory work.

Question 5 - State when the modifications were made

61. I do not know.

Question 6 - Identify those within the Laboratory responsible for the modifications

62. I do not know.

Question 7 - State the reasons why the modifications were made

.....
Generosa Lurdie

.....
Witness

63. I do not know.

2008 Report

Question 8 - Describe your role in the preparation of the 2008 Report

64. I did not have any role.

Question 9 - Describe the directions you received in relation to the preparation of the 2008 Report, and identify the person or persons from whom you received those directions.

65. I did not receive any directions.

Question 10 - State the substance of the communications (including discussions) that occurred between you, any other authors of the 2008 Report and/or any supervisor or person in a position of management concerning the purpose(s) or intended purpose(s) of the 2008 Report, including by identifying with whom those communications took place and when.

66. I do not recall having any communications about the 2008 Report.

Question 11 - Identify the persons to whom was the 2008 Report was distributed.

67. I do not know.

Question 12 - In relation to the matters stated in the 2008 Report, state:

Question 12(a) - how the conclusion on page 1 of the 2008 Report that "Data indicate that results from the automated procedure are comparable to those from the manual procedure" was reached, including:

- (i) any discussions or communications between any of the named authors of the 2008 Report and any supervisor or person in a position of management in relation to that conclusion or the referenced data; and
- (ii) how that conclusion can be reconciled with the data and figures outlined in part 6.4 of the 2008 Report.

68. I do not know. I do not recall being involved in the 2008 Report.

Question 12(b) - how the recommendations summarised on page 18 of the 2008 Report were decided, including by identifying:

- (i) your role in the decision;
- (ii) with whom and when you communicated (including by way of discussion) with any other person in connection with the recommendations and the decision to make them

69. I do not know. I do not recall being involved in the 2008 Report.

.....


Generosa Lündie



Witness

All the facts and circumstances declared in my statement, are within my own knowledge and belief, except for the facts and circumstances declared from information only, and where applicable, my means of knowledge and sources of information are contained in this statement.

I make this solemn declaration conscientiously believing the same to be true and by virtue of the provisions of the *Oaths Act 1867*.

TAKEN AND DECLARED before me at Brisbane on 24 October 2023

.....
[Redacted Signature]
Generosa Lundre

.....
[Redacted Signature]
Witness

EXHIBITS INDEX**Exhibits Index – Generosa Lundie Statement**

Question	Exhibit	Document Title
1(b)	GL-01	GENEROSA Jenny LUNDIE – CV
1(b)	GL-02	Project 9: Report on the Evaluation of Commercial DNA Extraction Chemistries 2007
1(b)	GL-03	Project 11: Report on Validation of a manual method for Extraction DNA using the DNA IQ System, August 2008
1(b)	GL-04	Chemical Validation of a Manual DNA Extraction Method using the DNA IQ System
1(b)	GL-05	Project 13. Report on the Verification of an Automated DNA IQ Protocol using the MultiPROBE II Plus HT ES with Gripper Integration Platform.

.....

 Generosa Lundie

.....

 Witness

GN-01

GENEROSA Jenny LUNDIE

E-mail: [REDACTED]

Mobile: [REDACTED]

Career Goals

Currently employed as a Scientist within the Evidence Recovery section of Forensic Biology at Forensic Science Queensland my goal is to continue utilising my scientific skills and experience in a team environment where Forensic DNA examination is the field of expertise.

To continue develop and advance my knowledge, understanding and contribute to the overall goals of the organisation.

Professional Experience

Scientist August 2003- Current
Evidence Recovery Section

Forensic Biology – Forensic Science Queensland*Responsibilities*

- Perform and record in accurate, concise, and contemporaneous manner, the examination of items submitted to Forensic Biology of items, in-tube items, and Forensic Medical Examination kits according to standard operating procedure.
- Entry and review of results examination into laboratory information system.
- Participate in internal and external proficiency testing as required.
- Maintain QIS event, participate in training and complete training modules.
- Provide training to scientists, technician or other staff as directed by the senior scientist.
- Maintenance of scientific knowledge and awareness of new/emerging technologies.

Scientist 2008-2003
Analytical Section

Forensic DNA Analysis- Forensic and Scientific Services Health Support Queensland*Responsibilities*

- Perform DNA extraction of casework and reference samples both automated and manual procedures using DNA IQ System and casework Pro kit for Maxwell 16.
- Perform DNA Quantification of extracted DNA using the Quant Studio Real-Time PCR System.
- Amplification of DNA extracts using PowerPlex21 on the Proflex thermal cyclers.
- Perform plate preparation of PCR products for capillary electrophoresis using 3500xl Genetic Analyzer.
- Interpretation of DNA profiles and CE Quality checking using Gene Mapper –IDX software for PowerPlex21.
- Import/upload results of reference and casework through Forensic Register.
- To ensure consistent production of quality results and assist in the maintenance of quality systems, monitor and update quality systems for example (raising of OQI's).
- Review, manage and validate results of samples and order rework strategy to obtain the best DNA profiles.
- Assist in the evaluation, verification and validation of new reagents, instruments, and equipment.
- Assist in the training of new staff member, when necessary, in analytical section.
- Perform maintenance and calibration of laboratory equipment and instrument such QIASymphony and Hamilton STARlet liquid handlers.
- Participate in a moot court training session
- To participate in staff and team meetings and take part in Performance Appraisal Development.
- Perform post-extraction processing of DNA extracts including Microcon, Nucleospin clean-ups, dilutions, and transfers and pooling.

GN-01

- Make standards for quantification of DNA extracts and testing of Quantifiler kits as well.
- Carry out weekly stock take and monthly environmental cleaning as well as general maintenance and cleaning of laboratory.
- Maintaining and updating relevant SOP's and all training requirements are up to date.
- Assist other team member in analytical area if needed, provided all the work required for the day has been completed.
- Ensure there's sufficient batches prepared both manual and automated procedures. Daily recording of Key Performance Index (KPI) for rostered area.
- Keep up to date of laboratory activities and changes by accessing meeting minutes, reading e-mail, Forensic Register Notification, AUSLAB system messages and newsletters.

Scientist 2006- 2008
Automation

Forensic DNA Analysis- Forensic and Scientific Services Health Support Queensland

Responsibilities

- Assist in the evaluation and validation of new DNA extraction kits for manual DNA extraction.
- Assist in the preparation of mock samples to be use in the validation of DNA extraction kits
- Perform operational procedures on the MP II Plus robotic platform including maintenance, gravimetric analysis, deck calibrations and setting-up for extraction processes.
- Use AUSLAB to register and batch functionality.
- Train and supervise staff in the operation of MP II Plus robotic platform using DNA IQ™ system.
- Participate in team meetings.

Laboratory Assistant March-June 2006
Operational Team

Forensic DNA Analysis- Forensic and Scientific Services Health Support Queensland

Responsibilities

- Perform FTA punching & washing to purify and amplify reference DNA samples.
- Perform blood clothing from reference and evidence sample received in the laboratory.
- Utilised AUSLAB for registration, storing, transfer of samples and batch functionality.
- Access QIS (Quality Information System) for updated protocols, QIS notifications and OQI (Opportunity for Quality Improvements).
- Assist in the environmental sampling and cleaning.
- To participate in staff and team meetings and take part in Performance Appraisal Development.

EDUCATIONAL QUALIFICATION

Bachelor of Biomedical Science

January 2003 - December 2005

Griffith University

Key Subjects

- Cell and Molecular Biology
- Biochemistry
- Laboratory Biotechniques
- Chemistry
- Biological Chemistry

GN-01

Bachelor of Science in Medical Technology

June 1985 - March 1991

Perpetual Help College of Medicine (Philippines)**Key subjects**

- Anatomy and Physiology
- Serology
- Hematology
- Parasitology
- Microbiology and Virology
- Immunology

Trainings

- Completion of the Perkin Elmer Users training for MPII Robotic Platform Workstation including (hardware overview, basic WinPREP Software, applications, specific training, customer preventive maintenance and good liquid handling.)
- Completed the training module in Interpretation and Acceptance of Results using AmpFISTR Profiler and Cofiler System™.
- Completed the training of Automated DNA IQ™ Method of Extracting DNA from Reference and Casework Samples.
- Completed the training in "Court Training" and Attendance at both Supreme and Magistrate Court.
- Processing FTA Paper™ using Profiler Plus.
- AUSLAB Functionality (Laboratory Information and Management System).
- Real Time PCR Quantification of Human DNA using Quantifiler Human DNA Quantification Kit.
- PCR Amplification using Profiler Plus and Cofiler System™.
- Competent to Train in the following modules (Operation, Maintenance and Gravimetric Analysis of the MPII Plus and Automated DNA IQ Method of Extracting DNA from Reference and Casework Samples using DNA IQ Kit.

SKILLS and ATTRIBUTES**Scientific knowledge and skills**

Gained through the completion of two medical science degrees, employment as a Scientist in Forensic DNA Analysis and as Medical Technician at Perpetual Hospital.)

Problem solving/trouble shooting

Developed through my involvement in various projects in DNA Analysis for which I participated/assisted in the validation to develop a new method of improving existing working practices.

Effective oral and written communications

Developed through regular interaction, meetings, and seminars attendance both internal and external. Assist in writing reports and updating Standard Operating Procedures.

Excellent teamwork skills

Through participation in team meetings, share information, contribute to all activities, and work co-operatively with team members to improve and achieve team performance and objectives.

GN-01

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Project 9: Report on the Evaluation of Commercial DNA Extraction Chemistries

2007

Automation and LIMS Implementation Project Team

DNA Analysis

Forensic And Scientific Services

Clinical and Scientific Services

Queensland Health

safe | sustainable | appropriate



Queensland Government
Queensland Health

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Project 9. Report on the Evaluation of Commercial DNA Extraction Chemistries

Breanna Gallagher[^], Vojtech Hlinka[^], Cecilia Iannuzzi[^], Generosa Lundle[^], Iman Muharam[^], Thomas Nuthen[^], Vanessa Ientile

[^] These authors contributed equally.

Automation/LIMS Implementation Project, DNA Analysis FSS (June 2007)

1. Abstract

DNA Analysis FSS performed an evaluation of various commercial DNA extraction chemistries in order to compare their overall performance (quality, yield, user-friendliness and the ability to automate) against the current in-house Chelex[®] protocol. Out of five commercial kits evaluated, the DNA IQ[™] system from Promega Corporation (Madison, WI, USA) was found to be the best out-of-the-box method for DNA extraction of blood and cell samples and will be validated for routine in-house use. This document presents data from the evaluation and provides a discussion of the results observed. For the manual DNA IQ[™] validation report, see Project 11. Verification of an automated DNA IQ[™] method is reported in Project 13.

2. Introduction

There have been many DNA extraction methods published since DNA was first isolated in 1953 (Butler, 2005). As technology developed and the demand for DNA testing increased, the methods for extracting and purifying DNA have improved. The Chelex[®] extraction procedure (Walsh *et al.*, 1991) became a quick and easy alternative to the more technically-demanding phenol/chloroform protocol and was more compatible for extracting samples from forensic exhibits, although the resulting DNA extract is still crude and unpurified because inhibitors are not removed from the solution. As the demand for extracting trace DNA samples has increased within the last 10 years to allow interrogation of low copy number forensic samples, coupled with the increase in the need to analyse difficult samples such as touched objects and degraded bone material, new DNA extraction technologies that are designed specifically for forensic samples have increased in availability.

The new DNA extraction chemistries on the market aim to overcome problems encountered in forensic DNA samples as they are designed to:

- Improve removal of inhibitors present in the sample that can affect DNA extraction (e.g. hemoglobin, textile dyes) or prevent successful PCR amplification (e.g. hematin, melanin, polysaccharides, bile salts, humic compounds);
- Maximise recovery of DNA in trace (low copy number) samples by using special buffers that promote cell lysis and integrating a DNA capture system that allows efficient binding and elution of sample DNA, therefore increasing total yields;
- Increase the overall quality and purity of recovered DNA by using special elution or storage buffers, therefore enhancing DNA stability for long-term storage, ensuring reliability and consistency in the sample DNA for reworks and future use.

DNA Analysis FSS obtained various commercial forensic DNA extraction kits (Table 1) in order to evaluate their performance against the in-house Chelex[®] protocol (see QIS 17171 for detailed information and literature on the Chelex[®] system).



Queensland Government
Queensland Health

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Table 1. Extraction kits that were evaluated by Forensic Biology FSS.

DNA extraction kit and manufacturer	Technology type
DNA IQ™ (Promega Corp., Madison, WI, USA)	Novel paramagnetic beads
QIAamp® DNA Micro (Qiagen GmbH, Hilden, Germany)	Silica-based membrane
ChargeSwitch® (Invitrogen, Carlsbad, CA, USA)	Magnetic beads
forensicGEM™ (ZyGEM, Hamilton, NZ)	Thermophilic proteinase incubation
NucleoSpin® 8 Trace (Macherey-Nagel, Düren, Germany)	Silica-based membrane

Magnetic bead technology is based on the use of magnetic resin that has the capability to bind DNA when subjected to a particular environmental pH or ionic strength. Therefore, by using buffers with different pH values or different ionic components, the binding and elution of DNA can be controlled. Furthermore, whilst the DNA is bound to the resin, the resin-DNA complex can be washed using an alcohol-containing buffer in order to remove inhibitors and residual proteins. A magnetic force is applied during the washing procedure to immobilise the resin-DNA complex and ensure no DNA is lost during washing. Membrane technology is based on a similar principle, except the DNA is immobilised in a thin silica-based membrane within the column.

forensicGEM™, the recently-released one-tube proteinase incubation system uses a thermostable enzyme to digest nucleases in order to yield a crude DNA extract. The enzyme digest method does not incorporate any washing steps, however, and therefore inhibitors are not removed from solution.

3. Aim

To evaluate several commercial DNA extraction kits (as per Table 1) that were specifically designed for forensic DNA samples, using the manufacturer's recommended manual protocols, and compare against the current in-house Chelex® protocol, in order to select a suitable kit for manual validation and automated verification.

4. Equipment and Materials

- Chelex® -100, P/N 143-2832 (Biorad, Hercules, CA, USA)
- DNA IQ™ System, P/N DC6701 (Promega Corp., Madison, WI, USA)
- QIAamp® DNA Micro Kit, P/N 56304 (Qiagen GmbH, Hilden, Germany)
- ChargeSwitch® Forensic DNA Purification Kit, P/N CS11200 (Invitrogen, Carlsbad, CA, USA)
- forensicGEM™ (ZyGEM, Hamilton, NZ)
- NucleoSpin® 8 Trace, P/N 740 722.1 (Macherey-Nagel, Düren, Germany)

For preparation of buffers and reagents specific for each kit, see the Methods section that is relevant for that kit.

5. Methods

5.1 Mock sample creation

Refer to document "Mock sample creation for cell and blood samples" (Gallagher *et al.*, 2007) for the detailed protocol.

CaSS | Forensic and Scientific Services

A CRIMINAL AND STATEWIDE SERVICE

5.2 DNA extraction kit protocols

The following section provides the principle and protocol for each DNA extraction kit as recommended by the manufacturer. The Chelex® method was as per QIS 17171.

5.2.1. Chelex®-100 (BioRad)

Principle

Chelex® is a chelating resin composed of styrene divinylbenzene copolymers which have a high affinity for polyvalent metal ions. The copolymers contain paired iminodiacetate ions acting as chelating groups which chelate metal ions, including some that degrade DNA while boiling the sample to obtain eluted DNA. Chelex® is the current Forensic Biology FSS standard in-house extraction protocol.

Equipment and Materials

- 20% Chelex® solution (w/v)
- Waterbath
- Magnetic stirrer plate
- 1.5mL sterile tubes
- Spin baskets
- Autoclaved nanopure water
- Vortex
- Centrifuge
- Twirling sticks
- Proteinase K (10mg/mL)
- FTA® Classic Card, P/N WB120205 (Whatman Plc)

Preparation of reagents

- 20% Chelex®-100

On balance, to a beaker containing a magnetic stirrer bar, add 2 grams of Chelex®-100 resin. To this, add 10mL of autoclaved nanopure water to make a 20% w/v solution and cover with parafilm. To ensure that the Chelex® is evenly dispersed, place beaker onto a magnetic stirrer plate before pipetting.

Methods (see QIS 17171R9)

1. Label sterile 1.5mL screw-capped tubes which contain sample as well as new elution tubes including extraction controls.
2. Pipette 1mL of autoclaved nanopure water into each tube, vortex gently.
3. Incubate at room temperature for 30 minutes.

The following steps are determined by sample type.

For Cells

4. For buccal FTA® punches, place tubes on multitube vortex for 5min at 12,000rpm.
5. For cell and/or fabric samples, twirl the substrate with a sterile twirling stick for 2min.

Note: Vortex FTA® punches samples then go to "For all sample types."

6. Transfer swab/fabric into spin baskets.
7. Spin tubes with spin basket for 30s at maximum speed (~15,800g or the applicable centrifuge's maximum setting). Discard spin basket with swab.

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

8. Vortex supernatant, then pour back into original extract tube.

For all sample types

9. Vortex, then spin in centrifuge for 3min at maximum speed (~15,800g or the applicable centrifuge's maximum setting).
10. Carefully remove all but 50µL of supernatant. Leave substrate in tube with pellet.
11. Add 150µL of 20% Chelex® to each tube and vortex.

Note: When pipetting Chelex, the resin beads must be distributed evenly in the solution. Use magnetic stirrer in beaker of Chelex and wide bore pipette tips.

12. Add 4µL of Proteinase K (10mg/mL) to cells and mix gently by vortexing.
13. Incubate in 56°C water bath for 30min for blood and cell samples.
14. Vortex until mixed, then incubate in boiling water bath for 8min.
15. Vortex until mixed, then centrifuge for 3min at maximum speed (~15,800g or the applicable centrifuge's maximum setting).
16. Transfer supernatant to new labelled 1.5mL screw-capped tube leaving Chelex® beads behind.
17. Samples are stored at -20°C.

5.2.2. DNA IQ™ System (Promega Corp.)

Principle

The Promega DNA IQ™ system for small casework samples incorporates two distinct steps. The first step provides an easy, rapid, efficient and almost universal cell lysis method to extract biological materials off stains on solid supports. The second step utilised a specific paramagnetic resin that purifies DNA without extensive washing to remove the lysis reagent. The DNA IQ™ system is designed to purify DNA samples approximately 100ng or less, and is more efficient with samples containing less than 10ng of DNA.

Equipment and Materials

- DNA IQ™ System (100 samples, Cat.# DC6701) containing:
 - 0.9mL Resin
 - 40mL Lysis Buffer
 - 30mL 2X Wash Buffer
 - 15mL Elution Buffer
- MagneSphere® Magnetic Separation Stand, 12-position (Cat.# Z5342)
- DNA IQ™ Spin Baskets (Cat.# V1221)
- Microtube 1.5mL (Cat.# V1231)
- 95-100% ethanol
- Isopropyl alcohol
- 1M DTT
- 65°C heat block
- 70°C heat block
- Vortex mixer

Preparation of Buffers

- *Preparing 1X Wash Buffer*
 - i. For DC6701 (100 samples), add 15mL of 95-100% ethanol and 15mL of isopropyl alcohol to 2X Wash Buffer.
 - ii. Replace cap and thoroughly mix by inversion.

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

- iii. Mark label to record addition of alcohols.
- iv. Label bottle as "1X Wash Buffer".
- v. Store bottle at room temperature with lid closed tightly to prevent evaporation.

• Preparing Lysis Buffer

- i. Determine the total amount of Lysis Buffer to be used (Table 2) and add 1µL of 1M DTT for every 100µL of Lysis Solution.

Table 2. Total amount of Lysis Buffer required for different sample material types.

Material	Lysis Buffer ¹	Lysis Buffer ²	Total Buffer
Liquid blood	100µL	100µL	200µL
Cotton swab	250µL	100µL	350µL
1/4 th CEP swab	250µL	100µL	350µL
15-50mm ² S&S 903 paper	150µL	100µL	250µL
3-30mm ² FTA [®] paper	150µL	100µL	250µL
Cloth up to 25mm ²	150µL	100µL	250µL

¹ For use in Step 2; ² For use in Step 9.

- ii. Mix by inversion.
- iii. Mark and date label to record addition of DTT.
- iv. Seal tube and store solution at room temperature for up to one month if required.

Method

DNA isolation from stains on solid material (non-liquid samples)

1. Place sample in a 1.5mL Microtube. The recommended amount of resin can capture a maximum of ~100ng DNA, therefore consider this when determining amount of sample to add.
2. Add 250µL of prepared Lysis Buffer (Table 2). Close lid and place on a 70°C heat block for 30min.
3. Remove tube from heat block and transfer the Lysis Buffer and sample to a DNA IQ™ Spin Basket.
4. Centrifuge at room temperature for 2min at maximum speed. Remove spin basket.
5. Vortex the stock Resin for 10s until it is thoroughly mixed. Add 7µL Resin to the sample. Keep the Resin resuspended while dispensing to obtain uniform results.
6. Vortex sample / Lysis Buffer / Resin mix for 3s. Incubate at room temperature for 5min.
7. Vortex for 2s and place tube in the MagneSphere® Magnetic Separation Stand. Separation will occur instantly.
8. Carefully remove and discard all of the solution without disturbing the Resin on the side of the tube.
9. Add 100µL of prepared Lysis Buffer. Remove the tube from the MagneSphere® Magnetic Separation Stand and vortex for 2 seconds.
10. Return tube to the MagneSphere® Magnetic Separation Stand and discard all Lysis Buffer, without disturbing the resin on the side of the tube.
11. Add 100µL prepared 1X Wash Buffer. Remove tube from the MagneSphere® Magnetic Separation Stand and vortex for 2s.
12. Return tube to the MagneSphere® Magnetic Separation Stand and discard all Wash Buffer, without disturbing the resin on the side of the tube.
13. Repeat steps 11 and 12 once for a total of 2 washes. Make sure that all of the solution has been removed after the last wash.



Queensland Government
Queensland Health

Page 5 of 34

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

14. With lid open, air-dry the Resin in the MagneSphere® Magnetic Separation Stand for 5min to 15min.
15. Add 25-100µL Elution Buffer, depending on how much biological material was used. A lower elution volume ensures a higher final concentration of DNA.
16. Close the lid, vortex the tube for 2s and incubate at 65°C for 5min.
17. Remove the tube from the heat block and vortex for 2s. Immediately place on the MagneSphere® Magnetic Separation Stand.
18. Transfer the solution to a fresh tube.
19. Store the DNA extract at 4°C for short-term storage or at -20 or -70°C for long term storage.

5.2.3. QIAamp® DNA Micro (Qiagen)

Principle

The QIAamp® DNA Micro kit combines selective binding properties of a silica-based membrane with flexible elution volumes that is suitable for a wide range of sample materials such as small volumes of blood, blood cards, small tissue samples and forensic samples. The basic procedure consists of 4 steps:

- Lysis: the sample is lysed;
- Bind: the DNA in the lysate binds to the membrane of the QIAamp® MinElute column;
- Wash: the membrane is washed;
- Elute: DNA is eluted from the membrane.

Equipment and Materials

- QIAamp® DNA Micro kit containing:
 - QIAamp® MinElute Columns;
 - collection tubes (2mL);
 - Buffer ATL;
 - Buffer AL;
 - Buffer AW1 (concentrate);
 - Buffer AW2 (concentrate);
 - Buffer AE;
 - carrier RNA (red cap);
 - Proteinase K.
- Ethanol (96-100%)
- 1.5mL or 2mL microcentrifuge tubes (for lysis steps)
- 1.5mL microcentrifuge tubes (for elution steps)
- Pipette tips
- Thermomixer
- Microcentrifuge with rotor for 2mL tubes
- Scissors
- Blood collection cards or FTA® card
- Sterile cotton swabs
- DTT

Important points before starting

- Perform all centrifugation steps at room temperature (15-25°C).
- Check whether carrier RNA is required; for purification of DNA from very small amounts of sample, such as low volumes of blood (<10µL) or forensic samples, it is recommended to add

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

carrier RNA to Buffer AL. For samples containing larger amounts of DNA, addition of carrier RNA is optional.

Steps to perform before starting

- Equilibrate Buffer AE or distilled water for elution to room temperature (15-25°C).
- Set a thermomixer or heated orbital incubator to 56°C for use in step 2, and a second thermomixer or heated orbital incubator to 70°C for use in step 5. If thermomixer or heated orbital incubators are not available, heating blocks or water baths can be used instead.
- If Buffer AL or Buffer ATL contains precipitates, dissolve by heating to 70°C with gentle agitation.
- If processing semen stains, hair, or nail clippings, prepare an aqueous 1M DTT (dithiothreitol) stock solution. Store aliquots at -20°C. Thaw immediately before use.
- Ensure that Buffers AW1 and AW2 have been prepared according to the instructions.

Preparation of Buffers

- **Preparing Buffer ATL**
Before starting the procedure, check whether precipitate has formed in Buffer ATL. If necessary, dissolve by heating to 70°C with gentle agitation.
- **Preparing Buffer AL**
Before starting the procedure, check whether precipitate has formed in Buffer AL. If necessary, dissolve by heating to 70°C with gentle agitation.
- **Preparing Buffer AW1**
Add 25mL ethanol (96-100%) to the bottle containing 19mL Buffer AW1 concentrate. Tick the check box on the bottle label to indicate that ethanol has been added. Reconstituted Buffer AW1 can be stored at room temperature (15-25°C) for up to 1 year. Note: before starting the procedure, mix the reconstituted Buffer AW1 by shaking.
- **Preparing Buffer AW2**
Add 30mL ethanol (96-100%) to the bottle containing 13mL Buffer AW2 concentrate. Reconstituted Buffer AW2 can be stored at room temperature (15-25°C) for up to 1 year. Note: before starting the procedure, mix the reconstituted Buffer AW2 by shaking.

Method

1. Lysing material stained with blood or saliva: cut out up to 0.5cm² of stained material and then cut into smaller pieces. Transfer the pieces to a 2mL microcentrifuge tube. Add 300µL buffer ATL, and 20µL Proteinase K. Close the lid and mix by pulse-vortexing for 10s. Continue this procedure from step 2.
2. Place the tube in a thermomixer or heated orbital incubator, and incubate at 56°C with shaking at 900rpm for at least 1hr. In general, hair is lysed in 1hr. If necessary, increase the incubation time to ensure complete lysis.
3. Briefly centrifuge the tube to remove droplets from the inside of the lid.
4. Add 300µL Buffer AL, close the lid, and mix by pulse vortexing for 10s. To ensure efficient lysis, it is essential that the sample and buffer AL are

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

thoroughly mixed to yield a homogeneous solution. A white precipitate may form when Buffer AL is added to buffer ATL. The precipitate does not interfere with the QIAamp® procedure and will dissolve during incubation in step 5. Note: if carrier RNA is required, add 1 µg dissolved carrier RNA to 300 µL buffer AL.

5. Place the tube in the thermomixer or heated orbital incubator, and incubate at 70°C with shaking at 900rpm for 10min. If using a heating block or water bath, vortex the tube for 10s every 3min to improve lysis.
6. Centrifuge the tube at full speed on a bench top centrifuge (20,000g; 14,000rpm) for 1min.
7. Carefully transfer the supernatant from step 6 to the QIAamp® MinElute column without wetting the rim. Close the lid, and centrifuge at 6,000g (8,000rpm) for 1min. Place the QIAamp® MinElute column in a clean 2mL collection tube, and discard the collection tube containing the flow-through.
8. If lysate has not completely passed through the membrane after centrifugation, centrifuge again at a higher speed until QIAamp® MinElute column is empty.
9. Carefully open the QIAamp® MinElute column and add 500 µL Buffer WA1 without wetting the rim. Close the lid and centrifuge 6,000g (8,000rpm) for 1min. Place the QIAamp® MinElute column in a clean 2mL collection tube and discard the collection tube containing the flow-through.
10. Carefully open the QIAamp® MinElute column and add 500 µL Buffer AW2 without wetting the rim. Close the lid and centrifuge at 6,000g (8,000rpm) for 1min. Place the QIAamp® MinElute column in a clean 2mL collection tube, and discard the collection tube containing the flow-through. Contact between the QIAamp® MinElute column and the flow-through should be avoided. Some centrifuge rotors may vibrate upon deceleration, resulting in the flow through, which contains ethanol, coming into contact with the QIAamp® MinElute column. Take care when removing the QIAamp® MinElute column and collection tube from the rotor, so that flow-through does not come into contact with the QIAamp® MinElute column.
11. Centrifuge at full speed (20,000g; 14,000rpm) for 3min to dry the membrane completely. This step is necessary, since ethanol carry-over into the eluate may interfere with some downstream applications.
12. Place the QIAamp® MinElute column in a clean 1.5mL microcentrifuge tube and discard the collection tube containing the flow through. Carefully open the lid of the QIAamp® MinElute column and apply 45 µL Buffer AE (equilibrated to room temperature) to the centre of the membrane to ensure complete elution of bound DNA. QIAamp® MinElute columns provide flexibility in the choice of elution volume.
13. Close the lid and incubate at room temperature (15-25°C) for 1min. Centrifuge at full speed (20,000g; 14,000rpm) for 1min. Incubating the QIAamp® MinElute columns loaded with Buffer AE or water for 5min at room temperature before centrifugation generally increases DNA yield.

5.2.4. ChargeSwitch® (Invitrogen)

Principle

ChargeSwitch® uses a novel magnetic bead-based technology known as ChargeSwitch Technology® (CST®). CST® provides a switchable surface charge, which is switched on and off by changing the pH. With a low pH buffer, the negatively charged DNA backbone binds to the positively charged beads and with a high pH buffer, DNA is eluted by neutralising the charge on the beads.



Queensland Government
Queensland Health

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

ChargeSwitch® uses a universal lysis step for all forensic sample types and has been designed to elute DNA from small sample volumes.

ChargeSwitch® uses a basic 4 step principle:

1. Lyse sample;
2. Negatively charged DNA binds to positively charged beads in a buffer with a pH ≤ 6 so charge is switched on;
3. At a pH of 7, charge is still on while beads and bound DNA is washed, removing any contaminants;
4. In a buffer with a pH of 8.5, charge is switched off and DNA is eluted from the beads.

Equipment and Materials

- o ChargeSwitch® Forensic DNA Purification kit (stored at room temperature) includes (for 100 preps):
 - o ChargeSwitch® Lysis Buffer (L13) – 100mL
 - o ChargeSwitch® Magnetic Beads (storage buffer: 10mM MES, pH 5.0; 10mM NaCl, 0.1% Tween 20) – 2 x 1mL
 - o Proteinase K (20mg/ml in 50mM Tris-HCl, pH 8.5, 5mM CaCl₂ 50% glycerol stored at 4°C) – 1mL
 - o ChargeSwitch® Purification Buffer (N5) – 20mL
 - o ChargeSwitch® Wash Buffer (W12) – 100mL
 - o ChargeSwitch® Elution Buffer (E5; 10mM Tris-HCl, pH 8.5) – 15mL
- o MagnaRack™, P/N CS15000 (Invitrogen)
- o Sterile, 1.5mL microcentrifuge tubes
- o Vortex mixer
- o Waterbath set at 55°C

Method

1. Set water bath at 55°C and prepare Lysis master mix in appropriate sized tube using the following formula: $n \times (1\text{mL ChargeSwitch® Lysis buffer} + 10\mu\text{L Proteinase K})$ where n is the number of samples.
2. To tube add 1mL of ChargeSwitch® Lysis Buffer (L13) and immerse forensic sample in mix.
3. Vortex/invert samples for 10-15s to mix then incubate in 55°C water bath for 1hr. Incubation can be shortened to 30min if sample is vortexed or inverted during this step.
4. Remove sample or transfer lysate to clean tube using 1mL pipette tips and pipette.
5. Vortex ChargeSwitch® Magnetic Beads to resuspend evenly in storage buffer.
6. Add 200 μL of ChargeSwitch® Purification Buffer (N5) to lysate and mix gently by pipetting up and down.
7. Add 20 μL of ChargeSwitch® Magnetic Beads to sample. Pipette-mix to ensure that no bubbles form.
8. Incubate for 1-5min at room temperature to allow the DNA to bind and then place sample tube in MagnaRack™ until a tight pellet has formed. Once this has occurred, aspirate supernatant from tube whilst still in rack and discard, ensuring that the pellet is not disturbed.
9. When supernatant has been completely discarded, remove tube from rack and add 500 μL ChargeSwitch® Wash Buffer (W12). Mix gently by pipetting up and down to resuspend the pellet.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

10. Allow beads to form a tight pellet by placing tube in MagnaRack™ and remove supernatant completely, without removing from rack or disturbing the pellet and discard.
11. Repeat steps 9 and 10 again.
12. Remove tube from rack, ensuring that supernatant has been completely removed and add 150µL ChargeSwitch® Elution Buffer (E5). Mix by pipetting up and down 10 times.
13. At room temperature, incubate for 1-5min then resuspend pellet and mix like in step 12.
14. Place tube in MagnaRack™ for 1min or until a tight pellet forms. Without removing tube from rack, aspirate DNA supernatant and place in a clean, sterile 1.5mL microcentrifuge tube, ensuring that the pellet is not disturbed. If elution is discoloured repeat steps 12 to 14 again.
15. Discard beads once extraction process is finished and either quantify immediately or store at -20°C.

5.2.5. *forensicGEM*™ (ZyGEM)

Principle

forensicGEM™ is a novel thermophilic proteinase developed as a rapid, cheap and effective DNA extraction solution for forensic laboratories that was recently released. It is a simple closed tube forensic DNA extraction method using a thermostable proteinase.

Protocols are available for blood and cell samples.

Equipment and Materials

- o *forensicGEM*™ buffer
- o *forensicGEM*™
- o Heat block or water bath set at 75°C and 95°C
- o 20µL sterile Aerosol Resistant Tips
- o 0.5-10µL pipettor
- o 300µL sterile Aerosol Resistant Tips
- o 20-200µL pipettor
- o 1mL sterile Aerosol Resistant Tips
- o 50µL-1mL pipettor

Method

DNA extraction from buccal swabs using *forensicGEM*™

1. Add buccal swab to tube.
Note: 1/4 head of swab specified but can utilise up to whole swab.
2. Add 200µL of *forensicGEM*™ buffer.
Note: if more than 1/4 head of buccal swab is used need to add more *forensicGEM*™ buffer. Moss *et al.* (2003) added 200µL more of the *forensicGEM*™ buffer for trace samples.
3. Add 2µL of *forensicGEM*™.
Note: *forensicGEM*™ buffer and *forensicGEM*™ can be added as a mastermix.
4. Incubate at 75°C for 15min.
5. Incubate at 95°C for 5min.
6. Remove supernatant to a new tube for storage.

DNA extraction from FTA® containing blood or saliva using *forensicGEM*™

1. UV irradiate plasticware for 5min.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

2. Add FTA® punches to each well of a 96-well plate.
Note: Larger punches can be added but not scalable SOP. PCR tubes can also be used for processing.
3. Add 100µL H₂O and leave at room temperature for 15min.
4. Decant water (remove by pipetting).
5. Add 100µL forensicGEM™ buffer and 2µL of forensicGEM™.
Note: The method is not listed as scalable.
6. Incubate at 75°C for 15min.
7. Incubate at 95°C for 5min.
8. Remove supernatant to a new tube for storage.

5.2.6. NucleoSpin® 8 Trace (Macherey-Nagel)

Principle

With the NucleoSpin® 8 Trace method, genomic DNA is prepared from forensic samples. Lysis is achieved by incubation of samples in a solution containing chaotropic ions in the presence of proteinase K at room temperature. Appropriate conditions for binding of DNA to the silica membrane in the NucleoSpin® 8 Trace Binding Strips are created by addition of isopropanol to the lysate. The binding process is reversible and specific to nucleic acids. Inhibitors are removed by two washing steps with ethanol buffer. Pure genomic DNA is finally eluted under low ionic strength conditions in a slightly alkaline elution buffer.

Equipment and Materials

- o NucleoSpin® 8 Trace kit, containing:
 - o Buffer FLB
 - o Buffer B5 (concentrate)
 - o Proteinase K (lyophilised)
 - o Proteinase Buffer
 - o Buffer BE
 - o NucleoSpin® 8 Trace Binding Strips
 - o MN Wash Plate
 - o MN Square-well Blocks
 - o MN Tube Strips
 - o Cap Strips
 - o Self-adhering PE Foil
- o NucleoSpin® 8 Trace Starter Set A containing Column Holders A and Dummy Strips
- o PVM vacuum manifold (from MultiPROBE® II PLUS HT EX platform)

Preparation of Buffers

- **Proteinase K**
Add 3mL Proteinase Buffer per vial to dissolve the lyophilised proteinase K and store at -20°C.
- **Buffer B5**
Add 160mL ethanol to 40mL Buffer B5.
- Store all other components of the kit at room temperature. Storage at lower temperatures may cause precipitation of salts. If a salt precipitate is observed, incubate the bottle at 30-40°C for a few minutes and mix well until all precipitation is redissolved.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Method

1. Premix 25µL Proteinase K and at least 125µL buffer FLB and add to sample. Incubate the sample at room temperature for 3 hours.
2. Insert spacers "MTP/Multi 96 plate" into the vacuum manifold. Place the waste container inside the vacuum manifold and insert a MN Wash Plate into the notches of the spacers. Close the manifold with the lid.
3. Place a NucleoSpin® Trace Binding Strips inserted in Column Holder A into the rubber seal of the vacuum manifold's lid and apply the samples to the wells of the plate.
4. Add 1 volume isopropanol to 2 volumes of lysate, mix three times and transfer to NucleoSpin® Trace Binding Strips.
5. Bind genomic DNA by applying vacuum until all lysates have passed through the columns (-200mbar 2min; -600mbar 10s). Ventilate the vacuum manifold.
6. Wash silica membrane by adding 900µL Buffer B5 to each well of the NucleoSpin® Trace Binding Strips. Apply vacuum (-200mbar 1min) until all buffer has passed through the columns. Ventilate the vacuum manifold.
7. Repeat the wash procedure once.
8. After the final washing step, close the valve, ventilate the vacuum manifold and remove the wash plate and waste container from the vacuum manifold.
9. Remove any residual washing buffer from the NucleoSpin® Trace Binding Strips. If necessary, tap the outlets of the NucleoSpin® Trace Binding Strips onto a clean paper sheet (supplied with the MN Wash Plate) or soft tissue until no drops come out. Insert the column holder with NucleoSpin® Trace Binding Strips into the lid and close the manifold. Apply maximum vacuum (-600mbar) for at least 10min to dry the membrane completely. This step is necessary to eliminate traces of ethanol. Close the valve and ventilate the vacuum manifold.
10. For elution, insert spacers "Microtube Rack" into manifold and rest rack with MN Tube Strips on spacers. Insert Column Holder A with NucleoSpin® Trace Binding Strips into manifold lid. Pipette 100µL Buffer BE directly to the bottom of each well and incubate for 5min at room temperature. Apply vacuum (-400mbar 2min).

5.3 DNA quantitation

All DNA extracts were quantified using the Quantifiler™ Human DNA Quantitation kit (Applied Biosystems, Foster City, CA, USA) as per QIS 19977. Reaction setup was performed on the MultiPROBE® II PLUS HT EX (PerkinElmer) pre-PCR platform.

5.4 PCR amplification and fragment analysis

DNA extracts were amplified using the AmpFISTR® Profiler Plus® kit (Applied Biosystems, Foster City, CA, USA) as per QIS 19976. Reaction setup was performed on the MultiPROBE® II PLUS HT EX (PerkinElmer) pre-PCR platform.

5.5 Capillary electrophoresis and fragment analysis

PCR product was prepared for capillary electrophoresis using the manual 9+1 protocol (refer to Project 15 and QIS 19978). Capillary electrophoresis was performed on an ABI Prism® 3100 Genetic Analyzer (Applied Biosystems, Foster City, CA, USA) under the following conditions: 3kV injection voltage, 10 sec injection time, 15kV run voltage, 100µA run current, and 45min run time. Data Collection Software version 1.1 was used to collect

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

raw data from the ABI Prism® 3100 Genetic Analyzer. Fragment size analysis was performed using GeneScan 3.7. Allele designation was performed using Genotyper 3.7, with thresholds for heterozygous and homozygous peaks at 150 and 300 RFU respectively. The allelic imbalance threshold is 70%.

6. Results and Discussion

6.1 Criteria for acceptance

Various commercial DNA extraction kits (as per Table 1) were evaluated in order to compare their performance against the current in-house Chelex® protocol. These kits were chosen because they were designed specifically for forensic samples and representative of the DNA capture technologies that were out on the market. Furthermore, these kits were manufactured by leaders in the field of DNA extraction technologies with a track record performance in supplying the forensic market with new and reliable products.

We assessed both magnetic bead and silica-based membrane technologies as the automated MultiPROBE® II platforms on which these systems will ultimately be operating on are fully compatible with both systems. The criteria against which the different kits were assessed on include:

1. *Total DNA yield*; the kit must yield sufficient DNA to perform multiple downstream tests such as DNA quantification and PCR amplification.
2. *Quality of the resulting DNA profiles*; the kit should be able to isolate DNA of a suitable quality for PCR amplification of STR loci, in order to generate DNA profiles that are suitable for forensic and human identification purposes.
3. *Ability to remove inhibitors*; the kit must be able to remove common inhibitors present in mock forensic samples (e.g. hemoglobin) using the basic manufacturer's procedure without the use of organic solvents.
4. *Usability*; the kit (and the manufacturer's recommended protocol) must be user-friendly. The necessary steps to prevent cross-contamination should also be described in the protocol. The extraction process should be able to be completed in a reasonable amount of time, comparable to the current procedure.
5. *Availability of validated forensic protocols*; the kit, including the manufacturer's protocol, must be validated for forensic use, either by the manufacturer or by a forensic laboratory, as determined from statements in the manufacturer's protocol or availability of publications in peer-reviewed journals.
6. *Availability of a validated MultiPROBE® II PLUS test file*; the kit should have a validated MPT file for use on the MultiPROBE® II PLUS HT EX platform.

Assessment of points 1, 2 and 3 was performed through experimentation. Point 4 was assessed based on operator feedback. This report provides results for points 1, 2, 3 and 4. A more extensive assessment of Point 3 was performed on the kit that was found to provide the best results for points 1, 2, 3 and 4 and is reported in Project 11. For points 5 and 6, the availability of validated protocols for all kits evaluated is outlined in Table 3.

The acceptance criteria were strictly adhered to in order to objectively evaluate the different systems. Out of all five DNA extraction technologies, there only existed a validated MultiPROBE® II PLUS test file for the DNA IQ™ system (Table 3). Although this was considered an advantage for DNA IQ™, we did not prematurely dismiss any of the other kits prior to evaluation. We decided that if a kit significantly outperformed the rest, and did not have a validated MPT file already created, that we would create a novel program file

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

with the kit manufacturer's assistance. This, however, would only be decided at the conclusion of the evaluation process.

Table 3. An assessment of available validated protocols for the various kits that were evaluated by Forensic Biology FSS.

Kit	Availability of validated forensic protocol	Availability of validated MP/II test file
DNA IQ™	✓	
QIAamp® DNA Micro	✓	
ChargeSwitch®	✓	x
forensicGEM™	✓	x
NucleoSpin® 8 Trace	✓	x

The results and discussion for each of the kits that were evaluated, in comparison to Chelex®, are provided in the following sections. Refer to Tables 4 and 5 for quantitation results for cell and blood samples respectively. Yield calculations for Chelex® samples assume a final elution volume of 150µL.

6.2 Evaluation of DNA IQ™

The DNA IQ™ system uses a novel paramagnetic resin for DNA isolation. It consists of two steps: (1) lysis of the biological material on solid support; (2) using the paramagnetic resin to bind DNA, which allows washing of the resin-DNA complex while the resin is immobilised by a magnetic force, in order to remove the lysis reagent and inhibitors in solution.

The manufacturer's method required the use of the MagneSphere® Magnetic Separation Stand. This magnetic stand is used for the separation of the magnetic pellet in 12 samples at a time. The time to process a batch of 12 samples using the DNA IQ™ system takes about 3 hours, including 30 minutes of incubation time.

Three controls were run with each extraction batch: (1) a negative extraction control (empty tube); (2) a positive extraction control (QC dot saliva or blood depending on the extraction); and (3) a substrate blank (the substrate with only saline).

Samples were extracted using the DNA IQ™ method as described in the Methods section and eluted using 100µL Elution Buffer. Due to volume loss during pipetting, the final elution volume is actually around 95µL. The same set of samples was also extracted using the in-house Chelex® protocol for comparison. Tables 4 and 5 display the DNA concentration (ng/µL) and yield (ng) for all cell and blood samples, compared to the results generated by Chelex®.



GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATISTICAL SERVICE

Table 4. Quantitation values for cell samples on different substrates after extraction by Chelex® and the evaluated DNA extraction kits.

Cells samples		Chelex		DNA IQ		QIAamp DNA Micro		ChargeSwitch		forensicGEM		NucliSens LT/Trace	
Sample ID	Substrate type	Concentration ng/μL	Yield ng	Concentration ng/μL	Yield ng	Concentration ng/μL	Yield ng	Concentration ng/μL	Yield ng	Concentration ng/μL	Yield ng	Concentration ng/μL	Yield ng
P5 (4uL, neat)	FTA	0.058800	11.877600	0.028700	2.870000	0.006030	0.271360	0.023900	3.585000	0.025700	2.821400	0.011500	1.820000
S5 (cotton) (4uL, neat)	Cotton swab	0.007410	1.111500	0.098000	9.800000	0.025800	1.161000	0.098700	14.505000	0.083300	18.826600	0.089000	6.890000
D5 (4uL, neat)	Cotton cloth	0.001480	0.222000	0.050700	5.070000	0.004880	0.219600	0.014900	2.235000	0.037400	7.500000	0.018000	7.180000
D5 (4uL, neat)	Denim cloth	0.002360	0.354000	0.028200	2.820000	0.002180	0.097200	0.003250	0.487500	0.041300	0.520000	0.035000	4.390000
R14_Neat 4uL	Rayon swab	0.016120	0.248000	0.018000	1.000000	0.000000	0.000000	0.011800	1.770000	0.024000	0.048000	0.031800	3.180000
R15_Neat 4uL	Rayon swab	0.015600	0.237000	0.019400	1.940000	0.005050	0.227250	0.018100	2.715000	0.019000	3.830000	0.115000	1.150000
R16_Neat 4uL	Rayon swab	0.000000	0.000000	0.015500	1.550000	0.006100	0.297450	0.027400	4.110000	0.010000	0.000000	0.057400	3.740000
R17_Neat 4uL	Rayon swab	0.000000	0.000000	0.011200	1.120000	0.007310	0.320950	0.009910	0.865300	0.019700	0.000000	0.029900	3.990000
Rayon mean (Neat)		0.000800	0.120000	0.014025	1.402500	0.004743	0.213413	0.016803	2.370376	0.018500	3.737000	0.038025	4.802500
Rayon STD (Neat)		0.000924	0.138586	0.004291	0.429137	0.003300	0.148490	0.009195	1.379299	0.005285	1.087463	0.039683	3.968338
F4 (4uL, 1/4 dilution)	FTA	0.010300	2.080600	0.005790	0.579000	0.005070	0.207150	0.007180	0.189000	0.007510	0.786020	0.005710	0.571000
S4 (cotton) (4uL, 1/4 dilution)	Cotton swab	0.000758	0.113400	0.019000	1.900000	0.001450	0.066600	0.031800	4.740000	0.008800	0.000000	0.000000	0.000000
C4 (4uL, 1/4 dilution)	Cotton cloth	0.000541	0.081150	0.015200	1.520000	0.000900	0.040900	0.000000	0.000000	0.011600	0.000000	0.000000	0.000000
D4 (4uL, 1/4 dilution)	Denim cloth	0.000000	0.000000	0.045800	4.580000	0.001600	1.881000	0.007120	0.258000	0.013400	2.708000	0.017600	7.000000
R10_1/4 4uL	Rayon swab	0.000358	0.037000	0.005740	0.574000	0.001800	0.681000	0.002880	0.429000	0.002950	0.000000	0.008760	0.876000
R11_1/4 4uL	Rayon swab	0.000000	0.000000	0.002560	0.256000	0.001300	0.058500	0.005150	0.922500	0.002020	0.000000	0.001220	0.122000
R12_1/4 4uL	Rayon swab	0.000058	0.134700	0.009750	0.975000	0.005370	0.250850	0.008560	0.984000	0.002340	0.000000	0.010200	0.020000
R13_1/4 4uL	Rayon swab	0.000433	0.054550	0.000000	0.000000	0.001550	0.089750	0.001350	0.202500	0.004030	0.000000	0.016000	1.600000
Rayon mean (1/4)		0.000472	0.070838	0.004513	0.451250	0.002655	0.114975	0.004230	0.634500	0.002835	0.0072670	0.008345	0.834500
Rayon STD (1/4)		0.000371	0.050697	0.004208	0.420706	0.002020	0.090915	0.002536	0.202328	0.004650	0.007801	0.009194	0.919400
F3 (4uL, 1/8 dilution)	FTA	0.008170	1.650340	0.008410	0.841000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000
S3 (cotton) (4uL, 1/8 dilution)	Cotton swab	0.003710	0.556300	0.012100	1.210000	0.001680	0.075800	0.009130	1.368500	0.000000	0.000000	0.014500	1.450000
C3 (4uL, 1/8 dilution)	Cotton cloth	0.002500	0.380000	0.010400	1.040000	0.000000	0.000000	0.009350	0.003260	0.000000	0.000000	0.006578	0.657000
D3 (4uL, 1/8 dilution)	Denim cloth	0.000739	0.110850	0.007630	0.763000	0.015100	0.875900	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000
R6_1/8 4uL	Rayon swab	0.000000	0.000000	0.001010	0.101000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000
R7_1/8 4uL	Rayon swab	0.000000	0.000000	0.000982	0.098200	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000
R8_1/8 4uL	Rayon swab	0.000000	0.000000	0.001540	0.154000	0.000000	0.000000	0.003380	0.508500	0.000000	0.000000	0.000000	0.000000
R9_1/8 4uL	Rayon swab	0.000739	0.110850	0.003050	0.305000	0.000000	0.000000	0.003360	0.504000	0.000000	0.000000	0.000000	0.000000
Rayon mean (1/8)		0.000785	0.077713	0.001846	0.184550	0.000000	0.000000	0.007862	0.279283	0.007355	0.316130	0.010033	1.003000
Rayon STD (1/8)		0.000370	0.035425	0.000971	0.097068	0.000000	0.000000	0.001770	0.765362	0.007807	0.385039	0.004200	0.420021
F2 (4uL, 1/16 dilution)	FTA	0.000000	0.000000	0.000000	0.000000	0.003940	0.177300	0.000000	0.000000	0.001940	0.000000	0.000000	0.000000
S2 (cotton) (4uL, 1/16 dilution)	Cotton swab	0.000000	0.000000	0.002900	0.290000	0.000000	0.000000	0.001520	0.228000	0.002260	0.000000	0.000000	0.000000
C2 (4uL, 1/16 dilution)	Cotton cloth	0.000000	0.000000	0.005010	0.501000	0.001870	0.094150	0.000000	0.000000	0.000741	0.149382	0.000000	0.000000
D2 (4uL, 1/16 dilution)	Denim cloth	0.000000	0.000000	0.002870	0.287000	0.000227	0.112150	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000
R2_1/16 4uL	Rayon swab	0.000000	0.000000	0.000717	0.071700	0.000000	0.000000	0.000000	0.000000	0.001200	0.244000	0.000000	0.000000
R3_1/16 4uL	Rayon swab	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000632	0.000000	0.000000	0.000000
R4_1/16 4uL	Rayon swab	0.000720	0.105000	0.002230	0.223000	0.000000	0.000000	0.003640	0.545000	0.002590	0.523100	0.004400	0.448000
R5_1/16 4uL	Rayon swab	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000000	0.000788	0.159776	0.000000	0.000000
Rayon mean (1/16)		0.000180	0.027000	0.000737	0.073675	0.000000	0.000000	0.000910	0.195560	0.001303	0.263705	0.002253	0.225333
Rayon STD (1/16)		0.000360	0.054000	0.001051	0.105131	0.000000	0.000000	0.001820	0.273000	0.000891	0.180012	0.002240	0.224012

GN-02

CaSS | Forensic and Scientific Services

CLINICAL AND RESEARCH SERVICE

Table 5. Quantitation values for blood samples on rayon swab substrates after extraction by Chelex® and the evaluated DNA extraction kits.

Blood samples	Chelex		DNA IQ		QIAamp DNA Micro		ChargeSwitch		foransicGEM		NucleoSpin 8 Trace	
Sample ID	Concentration ng/uL	Yield* ng	Concentration ng/uL	Yield ng	Concentration ng/uL	Yield ng	Concentration ng/uL	Yield ng	Concentration ng/uL	Yield ng	Concentration ng/uL	Yield ng
R14 (Neat)	2.37	355.5	0.482	48.2	2.31	103.85	0.751	112.65	0.00333	0.66266	1.16	116
R15 (Neat)	1.42	213	0.076	7.8	3.58	161.1	0.754	113.1	0.0068	1.3332	2.61	261
R16 (Neat)	0.512	76.8	0.356	35.6	3.32	149.4	0.929	139.35	0.0046	0.9292	1.61	161
R17 (Neat)	0.934	140.1	0.467	46.7	2.46	110.7	0.916	137.4	0.00727	1.46854	2.18	218
Mean (Neat)	1.3090	196.3500	0.3458	34.5750	2.9175	131.2875	0.8375	125.6250	0.0067	1.3534	1.8900	189.0000
STD (Neat)	0.7987	119.8085	0.1871	18.7137	0.8270	28.2137	0.0983	14.7451	0.0016	0.3173	0.6361	63.6082
R10 (1/4)	0.219	32.85	0.238	23.8	0.227	10.215	0.219	32.85	0.00211	0.42622	0.611	61.1
R11 (1/4)	0.0845	12.675	0.198	19.8	1.72	77.4	0.101	16.15	0.000597	0.20594	0.3	30
R12 (1/4)	0.216	32.4	0.195	19.5	4.59	206.55	0.0673	10.095	0.00128	0.25856	0.251	25.1
R13 (1/4)	0.165	24.75	0.136	13.6	0.657	29.565	0.0787	14.805	0.00156	0.33532	0.227	22.7
Mean (1/4)	0.1711	25.6688	0.1918	19.1750	1.7985	80.9325	0.1165	17.4750	0.00147	0.2852	0.3473	34.7250
STD (1/4)	0.0628	9.4262	0.0420	4.2019	1.5539	88.3776	0.0698	10.4628	0.0006	0.1294	0.1784	17.8438
R6 (1/8)	6.88	1032	0.0554	5.54	0.0936	4.212	0.094	14.1	0.0126	2.5452	0.154	15.4
R7 (1/8)	0.164	24.6	0.114	11.4	0.175	7.875	0.0735	11.025	0.00174	0.35148	0.148	14.8
R8 (1/8)	0.286	42.9	0.145	14.5	0.123	5.535	0.0521	7.815	0.00363	0.73326	0.178	17.8
R9 (1/8)	0.513	76.95	0.125	12.5	0.0151	0.6795	0.0939	14.085	0.00167	0.33734	0.0819	8.19
Mean (1/8)	1.9608	294.1125	0.1099	10.9850	0.1017	4.5754	0.0784	11.7563	0.00490	0.9918	0.1405	14.0475
STD (1/8)	3.2827	492.4030	0.0385	3.8501	0.0668	3.0068	0.0200	2.9991	0.0052	1.0517	0.0411	4.1145
R2 (1/16)	0.0405	6.075	0.0792	7.92	0.0349	1.5705	0.0347	5.205	0.00757	1.52374	0.0766	7.66
R3 (1/16)	0.0104	1.56	0.0566	5.66	0.0454	2.043	0.027	4.05	0.00667	1.34734	0.0923	9.23
R4 (1/16)	0.0337	5.055	0.0847	8.47	0.0386	1.737	0.0197	2.955	0.00544	1.09888	0.0588	5.88
R5 (1/16)	0.0323	4.845	0.109	10.9	0.0276	1.242	0.021	3.15	0.00245	0.4949	0.874	87.4
Mean (1/16)	0.0292	4.3838	0.0824	8.2375	0.0366	1.6481	0.0256	3.8400	0.0055	1.1175	0.2754	27.5425
STD (1/16)	0.0131	1.9577	0.0215	2.1515	0.0074	0.3341	0.0068	1.0274	0.0022	0.4510	0.3993	39.9285

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Comparison of quantitation results for cell samples

Refer to Table 4 for observed data. Using DNA IQ™, neat cell samples displayed higher quantitation results for both cotton and rayon swabs, and also for cotton and denim cloth materials. Only for the FTA® card was the result higher for the Chelex® sample. For 1/4 dilutions, DNA IQ™ results were higher than Chelex® results. For 1/8 dilutions, both protocols showed similar results for most sample types. Rayon swabs produced zero quantitation values for Chelex®, but exhibited consistent results for DNA IQ™. For 1/16 dilutions, most Chelex® samples were undetermined, whereas most DNA IQ™ samples yielded quantitation results.

Only three dilution samples extracted by DNA IQ™ gave zero quantitation values. In contrast, fourteen Chelex® samples gave zero quantitation results. This suggests that the DNA IQ™ sample recovery rate is 111% greater than that of the Chelex® protocol for cell samples.

Comparison of quantitation results for blood samples

Refer to Table 5 for observed data. For this experiment, only rayon samples (in quadruplicate) were tested. Neat blood samples showed higher concentration results when extracted using Chelex®. The 1/4 dilutions showed similar results for both methods. The 1/8 dilutions showed better results for Chelex®, but this was primarily due to an outlier result for one of the replicates (highlighted red in Table 4) that resulted in a concentration value 1300% greater than the remaining samples. This occurrence could be the result of inaccurate pipetting during mock sample creation or variability in the Chelex® method, specifically the inconsistent final elution volumes. For the 1/16 dilutions, the DNA IQ™ results were better. All DNA IQ™ results were more consistent and reproducible than Chelex® results.

Overall, samples that were extracted using DNA IQ™ showed quantitation results that were similar to or better than samples that were extracted using Chelex®. For cell substrates, 44% of Chelex® samples gave zero quantitation results, compared to only 9% for DNA IQ™ samples. All blood substrates generated quantitation results that were similar for both methods. Furthermore, DNA IQ™ generated results that were more sensitive, consistent and reproducible across multiple replicates.

Comparison of DNA profiles

Cell samples that were extracted using the DNA IQ™ method gave DNA profiles with more alleles compared to extractions performed using Chelex® (Table 6). Overall, DNA IQ™ resulted in 282 reportable alleles (excluding Amelogenin), compared to 89 alleles resolved by Chelex®, or in other words samples extracted using DNA IQ™ generated 216% more reportable alleles compared to samples extracted using Chelex®. For neat cell substrates, DNA IQ™ samples generated full profiles in all instances except 2: an X,X+14 for the FTA® substrate and an X,X+16 for a rayon swab replicate. All rayon samples extracted by Chelex® did not produce any profiles at all, in contrast to the full profile results using DNA IQ™. DNA IQ™ also gave more reportable alleles for the lower dilutions compared to Chelex®. Additionally, DNA IQ™ was able to yield full profiles from denim substrates, compared to Chelex® which yielded no profiles at all. This observation indicates the superiority of the DNA IQ™ system for removing and overcoming inhibition due to denim dye. Only one occurrence of allelic imbalance (68% at D13S317) was encountered in all 64 samples.



Queensland Government
Queensland Health

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Table 6. Comparison of DNA profiles for cell substrate samples extracted using either Chelex® or DNA IQ™.

CELLS Method: Chelex							CELLS Method: DNA IQ						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim		Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
	Profile	Profile	Sample#	Profile	Profile			Profile	Profile	Sample#	Profile	Profile	
Neat	XX+18	XX+18	R14	NSD	XX+8	NR/NSD	Neat	XX+14	XX+18	R14	XX+18	XX+18	XX+18
			R16	NR/NSD						R16	NR/NSD		
			R17	NSD						R17	XX+18		
			R17	NSD						R17	XX+18		
Dil 1/4	XX+18	XXNR+3	R10	NSD	NR+1	NR/NSD	Dil 1/4	XX+17	XX+18	R10	NR+3	XX+18	XX+18
			R11	NSD						R11	NR/NSD		
			R12	NSD						R12	XX+6		
			R13	NSD						R13	NR/NSD		
Dil 1/8	XX+17	XX+3	R6	NSD	XXNR+3	NR/NSD	Dil 1/8	XX+8	XX+18	R6	NR/NSD	XX+17	XX+17
			R7	NSD						R7	NR/NSD		
			R8	NSD						R8	NR/NSD		
			R9	NSD						R9	NR/NSD		
Dil 1/16	NSD	NSD	R2	NSD	NSD	NSD	Dil 1/16	NSD	XX+4	R2	NR/NSD	NR/NSD	NR/NSD
			R3	NSD						R3	NSD		
			R4	NSD						R4	NR/NSD		
			R5	NSD						R5	NSD		

For blood samples, only rayon substrates were extracted using the DNA IQ™ system as these were deemed sufficient for observing the effects of heme inhibition (without the need to factor variable substrate types). Almost all samples generated full profiles or a sufficient number of reportable alleles for matching purposes (Table 7). For neat samples extracted by Chelex®, no profiles were resulted from the FTA®, cotton swab or denim samples, indicating possible heme inhibition that could not be removed by the Chelex® protocol. For rayon samples, 19% of those extracted by Chelex® did not generate a profile, whereas DNA IQ™ yielded full profiles for all dilutions except two neat samples. Reworks of the two failed samples were performed but yielded the same NSD results. These failed results appear to be outliers, as all other dilutions yielded the expected results. It was observed that results from blood samples on rayon swabs were more likely (32%) to exhibit allelic imbalance at Amelogenin when extracted using the DNA IQ™ system.

Table 7. Comparison of DNA profiles for blood substrate samples extracted using either Chelex® or DNA IQ™.

BLOOD Method: Chelex							BLOOD Method: DNA IQ						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim		Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
	Profile	Profile	Sample#	Profile	Profile			Profile	Profile	Sample#	Profile	Profile	
Neat	NSD	NSD	R14	XY+18	XY+18	NSD	Neat	NSD	NSD	R14	NSD		
			R15	XY+18						R15	NSD		
			R18	XY+18						R16	XY+18(AI@AMEL)		
			R17	NR/NSD						R17	XY+18(AI@AMEL)		
Dil 1/4	XY+18	XY+15	R10	Not Uploaded	XY+18	XY+18	Dil 1/4	XY+18	XY+18	R10	XY+18		
			R11	XY+18						R11	XY+18(AI@AMEL)		
			R12	XY+18						R12	XY+18		
			R13	XY+18						R13	XY+18		
Dil 1/8	XY+18(AI@AMEL)	XY+18	R6	XY+18	XY+18	XY+18	Dil 1/8	XY+18(AI@AMEL)	XY+18	R6	XY+18(AI@AMEL)		
			R7	XY+18						R7	XY+18		
			R8	NR/NSD						R8	XY+18		
			R9	XY+18						R9	XY+18		
Dil 1/16	XY+18	XY+18	R2	XY+18	XY+18	XY+18	Dil 1/16	XY+18	XY+18	R2	XY+18(AI@AMEL)		
			R3	XY+18						R3	XY+18		
			R4	XY+18						R4	XY+18		
			R5	XY+18						R5	XY+18		

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

We found the DNA IQ™ system yielded results that were either comparable or better than results generated by samples extracted using the in-house Chelex® protocol, both in terms of quantitation values and DNA profile quality and completeness.

6.3 Evaluation of QIAamp® DNA Micro

The QIAamp® DNA Micro kit was designed for the purification of genomic and mitochondrial DNA from small sample volumes or sizes, as often encountered in forensics. The system uses a silica-based membrane to accommodate DNA binding and purification using special buffers, followed by elution in buffer or water, resulting in purified DNA that is free of proteins, nucleases and other impurities.

The QIAamp® DNA Micro system consists of four steps: lysing, binding, washing, followed by elution:

- **Lysis** – Small samples are lysed under highly denaturing conditions at elevated temperatures under the presence of Proteinase K.
- **Binding** – Using Buffer AL and ethanol, DNA is adsorbed into the silica-gel membrane of the column by centrifugation or application of a vacuum. The buffer is formulated so that proteins and other components are not retained in the membrane.
- **Washing** – While DNA is bound to the silica membrane, contaminants are efficiently washed away using a combination of two wash buffers.
- **Elution** – DNA is eluted in a small volume of Buffer AE or sterile water, yielding concentrated DNA.

The QIAamp® protocol involves 5 tube transfers and therefore takes approximately 5 hours to perform a manual extraction of 12 samples. The same set of samples that were used for the DNA IQ™ evaluation was also used to evaluate QIAamp® DNA Micro. Each extraction batch included a positive and negative control, and also a substrate blank. DNA was eluted in 45µL volume.

Comparison of quantitation results for cell samples

Refer to Table 4 for observed data. Twelve samples extracted by QIAamp® gave zero quantitation values, compared to fourteen samples by Chelex®. Despite the low elution volume of 45µL in the QIAamp® protocol that serves to concentrate the purified DNA, quantitation results for all samples were comparable for both DNA extraction methods.

Comparison of quantitation results for blood samples

Refer to Table 5 for observed data. Blood on rayon swab samples displayed wide variation between replicates. For neat samples, the total yield is comparable to Chelex®, however, lower dilutions (1/8 – 1/16) suffer from inconsistencies. One of the 1/4 dilution replicates displayed an unexpectedly high quantitation value that was more than 3x greater than the Chelex® average yield, but this can be attributed to inaccurate pipetting, or pipetting of a non-uniform sample mixture, during mock sample creation.

A possible reason as to why the quantitation results for both cell and blood samples were inconsistent is because the QIAamp® DNA Micro protocol uses five sets of collection tubes for supernatant transfer, therefore possibly causing sample lost during multiple sample transfers from one tube to another.



Queensland Government
Queensland Health

CaSS | Forensic and Scientific Services

A CLINICAL AND STATISTICAL SERVICE

Comparison of DNA profiles

Cell samples that were extracted using the QIAamp® protocol showed profile results that were either comparable or worse than samples that were extracted using the Chelex® protocol (Table 8). Out of 32 samples, only one QIAamp® sample resulted in a full profile (X,X+18). QIAamp® samples failed to produce full profiles for all but one (n = 8) of the neat samples. Overall, QIAamp® resulted in 86 reportable alleles compared to 89 alleles resolved by Chelex®. Some of the QIAamp® allele calls are inconsistent, e.g. the result for 1/4 dilution on cotton cloth was slightly better than the neat sample. This is further exemplified by the denim substrate samples. The QIAamp® method did not appear to effectively overcome inhibition caused by the denim dye as observed from the resulting profiles.

Table 8. Comparison of DNA profiles for cell substrate samples extracted using either Chelex® or QIAamp® DNA Micro.

CELLS Method: Chelex							CELLS Method: QIAamp DNA Micro						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim		Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
	Profile	Profile	Sample#	Profile	Profile	Profile		Profile	Profile	Sample#	Profile	Profile	Profile
Neat	XX+18	XX+18	R14	NSD	XX+8	NR/NSD	Neat	XX+12	XX+10	R15	NSD	NR, NR+2	NR/NSD
			R15	NR/NSD						R16	NR/NSD		
			R16	NSD						R17	NR/NSD		
			R17	NSD						R18	NR/NSD		
Dil 1/4	XX+18	XXNR+3	R10	NSD	NR+1	NR/NSD	Dil 1/4	XX+14	XX+15	R10	NSD	NR, NR+3	NR/NSD
			R11	NSD						R11	NSD		
			R12	NSD						R12	NR/NSD		
			R13	NSD						R13	NR/NSD		
Dil 1/8	XX+17	XX+3	R6	NSD	XXNR+3	NR/NSD	Dil 1/8	NSD+2	XXNR+6	R6	NSD	NR/NSD	NR+7
			R7	NSD						R7	NSD		
			R8	NSD						R8	NSD		
			R9	NSD						R9	NSD		
Dil 1/16	NSD	NSD	R2	NSD	NSD	NSD	Dil 1/16	NR/NSD	NR/NSD	R2	NSD	NSD	NSD
			R3	NSD						R3	NSD		
			R4	NSD						R4	NSD		
			R5	NSD						R5	NSD		

Table 9. Comparison of DNA profiles for blood substrate samples extracted using either Chelex® or QIAamp® DNA Micro.

BLOOD Method: Chelex							BLOOD Method: QIAamp DNA Micro						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim		Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
	Profile	Profile	Sample#	Profile	Profile	Profile		Profile	Profile	Sample#	Profile	Profile	Profile
Neat	NSD	NSD	R14	XY+18	XY+18	NSD	Neat	NSD	NSD	R14	XY+18	XY+18	XY+18
			R15	XY+18						R15	XY+18		
			R16	XY+18						R16	XY+18		
			R17	NR/NSD						R17	NR, Y+15		
Dil 1/4	XY+18	XY+15	R10	Not Uploaded	XY+18	XY+18	Dil 1/4	XY+18	XY+15	R10	XY+18		
			R11	XY+18						R11	XY+17		
			R12	XY+18						R12	XY+18		
			R13	XY+18						R13	XY+18		
Dil 1/8	XY+18(AI@D)	XY+18	R6	XY+18	XY+18	XY+18	Dil 1/8	XY+18(AI@D)	XY+18	R6	XY+18		
			R7	XY+18						R7	XY+18		
			R8	NR/NSD						R8	XY+18		
			R9	XY+18						R9	XY+18		
Dil 1/16	XY+18	XY+18	R2	XY+18	XY+18	XY+18	Dil 1/16	XY+18	XY+18	R2	XY+18(AI@D8,D18)		
			R3	XY+18						R3	XY+18		
			R4	XY+18						R4	XY+18		
			R5	XY+18						R5	XY+18		

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

For blood samples on rayon swabs, 87.5% of QIAamp® samples resulted in full profiles, compared to 81.25% of Chelex® samples (Table 9). Out of all QIAamp® rayon swab samples, only one of the 1/16 replicates displayed allelic imbalance (in D8S1179 and D18S51).

6.4 Evaluation of ChargeSwitch®

The ChargeSwitch® technology (CST) is another magnetic bead-based technology that provides a switchable surface charge dependent on the pH of the surrounding buffer environment to facilitate DNA isolation from small forensic samples. In low pH conditions the ChargeSwitch® beads have a positive charge that allows negatively charged DNA to bind. In this environment, proteins and other contaminants are not bound and can be washed away. By using a low salt elution buffer at pH 8.5, the charge on the bead surface is neutralised and DNA can be eluted for immediate use in downstream forensic applications.

The ChargeSwitch® Elution Buffer (E5) that is supplied with the kit is used to provide an environment with a pH of 8.5 that promotes dissociation of bound DNA from the magnetic beads and therefore efficient elution of purified DNA. However, TE buffer with a pH between 8.5 – 9.0 can also be used for elution. TE buffer outside of this pH range should not be used. The use of water for elution is also not recommended.

The manufacturer's method required the use of the MagnaRack™ two-piece magnetic separation rack that consists of two components: a magnetic base station and removable tube rack. The tube rack holds up to 24 microcentrifuge tubes and fits onto the magnetic base station in two different positions associating the row of 12 neodymium magnets with a single row of 12 tubes for simple 'on the magnet' and 'off the magnet' processing. The time to process a batch of 12 samples using the ChargeSwitch® system takes about 3.5 hours, including 30 minutes of incubation time. Each extraction batch included a positive and negative control, and also a substrate blank. Purified DNA samples were eluted in 150µL Elution Buffer (E5).

Comparison of quantitation results for cell samples

Refer to Table 4 for observed data. For cell samples, ChargeSwitch® performed moderately better compared to the current in-house Chelex® method. When comparing the quantitation values, ChargeSwitch® produced higher quantitation values for cotton and rayon swabs over all dilutions as well as the neat samples of cotton shirt and denim jeans. For other cell samples, ChargeSwitch® performance was comparable to the Chelex® results.

Comparison of quantitation results for blood samples

Refer to Table 5 for observed data. ChargeSwitch® quantitation results for blood samples on rayon swabs were lower but more consistent than Chelex® results.

Comparison of DNA profiles

Cell samples that were extracted using the ChargeSwitch® system showed profile results that were comparable to samples that were extracted using the Chelex® protocol (Table 10). Overall, ChargeSwitch® resulted in 138 reportable alleles compared to 89 alleles resolved by Chelex®. ChargeSwitch® performance for cell samples on FTA® cards was poor for any samples less than the neat dilution. Profiles for both cotton swab and cotton cloth samples were slightly better for ChargeSwitch®, and results for neat samples on rayon

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

swabs outperformed Chelex[®]. However, the ChargeSwitch[®] system was unable to overcome inhibition in denim samples, and did not yield any DNA profiles at all, despite displaying quantitation results for the neat and 1/4 dilution.

Table 10. Comparison of DNA profiles for cell substrate samples extracted using either Chelex[®] or ChargeSwitch[®].

CELLS Method: Chelex							CELLS Method: ChargeSwitch						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim			FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
	Profile	Profile	Sample#	Profile	Profile	Profile		Profile	Profile	Sample#	Profile	Profile	Profile
Neat	XX+18	XX+18	R14	NSD	XX+8	NR/NSD		XX+17	XX+18	R14	XX+8	XX+11	NSD
			R16	NR/NSD						R15	XX+18		
			R18	NSD						R16	XX+18		
			R17	NSD						R17	XX+18		
DI 1/4	XX+18	XX+3	R10	NSD	NR+1	NR/NSD		XX+9	XX+18	R10	XX+NR+1	NRNR+2	NSD
			R11	NSD						R11	NR/NSD		
			R12	NSD						R12	XXNR+2		
			R13	NSD						R13	XXNR+NSD		
DI 1/8	XX+17	XX+3	R6	NSD	XXNR+3	NR/NSD		NR/NSD	XX+18	R6	NSD	NR/NSD	NSD
			R7	NSD						R7	NSD		
			R8	NSD						R8	NR/NSD		
			R9	NSD						R9	NSD		
DI 1/16	NSD	NSD	R2	NSD	NSD	NSD		NSD	NR/NSD	R2	NR/NSD	NSD	NSD
			R3	NSD						R3	NSD		
			R4	NSD						R4	NSD		
			R5	NSD						R5	NSD		

For blood samples on rayon swab substrates, all ChargeSwitch[®] samples consistently yielded full profiles for all dilutions and therefore outperformed Chelex[®] (Table 11). Two replicates of the lower, 1/16 dilutions displayed allelic imbalance at two different loci: D3S1358 and D7S820, possibly due to stochastic effects that arise from amplifying low concentrations of DNA.

Table 11. Comparison of DNA profiles for blood substrate samples extracted using either Chelex[®] or ChargeSwitch[®].

BLOOD Method: Chelex							BLOOD Method: ChargeSwitch						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim			FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
	Profile	Profile	Sample#	Profile	Profile	Profile				Sample#	Profile	Profile	Profile
Neat	NSD	NSD	R14	XY+18	XY+18	NSD				R14	XY+18		
			R15	XY+18						R15	XY+18		
			R16	XY+18						R16	XY+18		
			R17	NR/NSD						R17	XY+18		
DI 1/4	XY+18	XY+15	R10	Not Uploaded	XY+18	XY+18				R10	XY+18		
			R11	XY+18						R11	XY+18		
			R12	XY+18						R12	XY+18		
			R13	XY+18						R13	XY+18		
DI 1/8	XY+18(AI@D3)	XY+18	R6	XY+18	XY+18	XY+18				R6	XY+18		
			R7	XY+18						R7	XY+18		
			R8	NR/NSD						R8	XY+18		
			R9	XY+18						R9	XY+18		
DI 1/16	XY+18	XY+18	R2	XY+18	XY+18	XY+18				R2	XY+18		
			R3	XY+18						R3	XY+18		
			R4	XY+18						R4	XY+18(AI@D3)		
			R5	XY+18						R5	XY+18(AI@D7)		

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

6.5 Evaluation of *forensicGEM*TM

*forensicGEM*TM is a novel thermostable proteinase developed as a rapid, cheap and effective single-tube DNA extraction solution for forensic laboratories that was recently released. At the time of testing, the *forensicGEM*TM system was not yet widely used in the field of forensics, however the system has had exposure at various conferences and symposiums, such as the 18th International Symposium on the Forensic Sciences (Fremantle, WA; 2-7 April 2006).

Unlike the other kits that were evaluated, *forensicGEM*TM does not incorporate either magnetic-bead or silica membrane technologies, but instead works on the principle of action of a thermostable proteinase in an optimised buffer solution. *forensicGEM*TM is based on the work of Moss *et al.* (2003) who developed the use of EA1 proteinase for the DNA extraction of forensic samples. EA1 proteinase comes from the thermophilic *Bacillus* sp. EA1. EA1 proteinase is Ca²⁺ dependent but is unaffected by a concentration of citrate below 5mM and EDTA below 2mM (Moss *et al.* 2003). For EDTA-stabilised blood, the buffer needs to be supplemented to a final concentration of 200µM CaCl₂. Heating a sample at 75°C in the presence of *forensicGEM*TM buffer and *forensicGEM*TM lyses the sample and the proteinase hydrolyses nucleases. At 95°C the proteinase is heat-inactivated so that an active form will not be carried over into PCR where it would degrade Taq DNA polymerase.

The time to process a batch of 12 samples using the *forensicGEM*TM system takes about 1.5 hours. Each extraction batch included a positive and negative control, and also a substrate blank. The final volume was 100µL for FTA[®] samples and 200µL for all other samples.

Comparison of quantitation results for cell samples

Refer to Table 4 for observed data. For cells samples, *forensicGEM*TM produced higher quantitation results compared to Chelex[®] across all dilutions. *forensicGEM*TM also generated the highest yield for all samples, including the 1/16 dilutions. *forensicGEM*TM yielded quantitation results for denim samples (neat and 1/4 dilutions).

Comparison of quantitation results for blood samples

Refer to Table 5 for observed data. *forensicGEM*TM performed very poorly for blood samples on rayon swabs, resulting in the lowest observed yield across all kits that were evaluated. The average yield for all four neat replicates processed using *forensicGEM*TM was 0.6% of the average yield for all Chelex[®] replicates. The best average yield results were observed for 1/16 dilution samples, where the average *forensicGEM*TM yield was around 25% that of Chelex[®]. This suggests that the *forensicGEM*TM system is prone to heme inhibition if a neat sample is processed, but can slightly overcome the inhibitory effect if the blood sample is diluted prior to extraction.

Comparison of DNA profiles

*forensicGEM*TM resulted in 209 reportable alleles for cell samples compared to 89 alleles resulting from Chelex[®] extracts (Table 12). *forensicGEM*TM was able to overcome inhibition in denim samples, producing full profiles (X,X+18) for neat and 1/4 dilutions, accurately reflecting the quantitation results. A partial profile (X,NR+7) was obtained for the 1/8 dilution on denim. *forensicGEM*TM results were also superior than Chelex[®] for cells on cotton swab down to the 1/8 dilution, but FTA[®] results were considerably poor.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Table 12. Comparison of DNA profiles for cell substrate samples extracted using either Chelex® or forensicGEM®.

CELLS Method: Chelex							CELLS Method: forensicGEM						
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim			FTA	Cotton swabs	Rayon swabs	Cotton	Denim	
Profile	Profile	Sample#	Profile	Profile	Profile		Profile	Profile	Sample#	Profile	Profile	Profile	
Neat	XX+16	XX+16	R14	NSD	XX+8	NR/NSD	Neat	XX+16	XX+16	R14	XX+16	XX+16	XX+16
			R16	NR/NSD						R16	XX+16	XX+16	XX+16
			R16	NSD						R16	XX+16	XX+16	XX+16
			R17	NSD						R17	XX+16	XX+16	XX+16
DI 1/4	XX+16	XX+3	R10	NSD	NR+1	NR/NSD	DI 1/4	XX+3	XX+16	R10	XX+3	XX+16	XX+16
			R11	NSD						R11	NR/NSD	NR/NSD	NR/NSD
			R12	NSD						R12	NR/NSD	NR/NSD	NR/NSD
			R13	NSD						R13	NR/NSD	NR/NSD	NR/NSD
DI 1/8	XX+17	XX+9	R8	NSD	XX+9	NR/NSD	DI 1/8	NSD	XX+16	R7	NR/NSD	XX+10	XX+7
			R7	NSD						R8	NSD	NSD	NSD
			R8	NSD						R9	NR/NSD	NR/NSD	NR/NSD
			R9	NSD						R6	NR/NSD	NR/NSD	NR/NSD
DI 1/16	NSD	NSD	R2	NSD	NSD	NSD	DI 1/16	NSD	NR/NSD	R6	NSD	NSD	NR/NSD
			R3	NSD						R4	NSD	NSD	NSD
			R4	NSD						R3	NSD	NSD	NSD
			R5	NSD						R2	NR/NSD	NR/NSD	NR/NSD

For blood samples on rayon swabs, only the 1/16 dilutions generated profile results (Table 13). This is indicative of potential inhibition for higher blood sample dilutions as predicted by the quantitation data.

Table 13. Comparison of DNA profiles for blood substrate samples extracted using either Chelex® or forensicGEM®.

BLOOD Method: Chelex										BLOOD Method: forensicGEM									
Dilution	FTA	Cotton swabs	Rayon swabs	Cotton	Denim	Rayon swabs					FTA	Cotton swabs	Rayon swabs	Cotton	Denim	Rayon swabs			
Profile	Profile	Sample#	Profile	Profile	Profile	Sample#	Profile	Profile	Sample#	Profile	Profile	Sample#	Profile	Profile	Sample#	Profile	Profile	Sample#	Profile
Neat	NSD	NSD	R14	XY+16	XY+16	NSD	R14	NSD	NSD	Neat	NSD	NSD	R14	XY+16	XY+16	NSD	NSD	NSD	NSD
			R15	XY+16			R15	NSD	NSD				R15	XY+16			NSD	NSD	NSD
			R16	XY+16			R16	NSD	NSD				R16	XY+16			NSD	NSD	NSD
			R17	NR/NSD			R17	NSD	NSD				R17	XY+16			NSD	NSD	NSD
DI 1/4	XY+16	XY+16	R10	Not Uploaded	XY+16	XY+16	R10	NSD	NSD	DI 1/4	XY+16	XY+16	R10	XY+16	XY+16	NSD	NSD	NSD	NSD
			R11	XY+16			R11	NSD	NSD				R11	XY+16			NSD	NSD	NSD
			R12	XY+16			R12	NSD	NSD				R12	XY+16			NSD	NSD	NSD
			R13	XY+16			R13	NSD	NSD				R13	XY+16			NSD	NSD	NSD
DI 1/8	XY+16(A)@XY+16		R6	XY+16	XY+16	XY+16	R6	NSD	NSD	DI 1/8	XY+16(A)@XY+16		R6	XY+16	XY+16	NSD	NSD	NSD	NSD
			R7	XY+16			R7	NSD	NSD				R7	XY+16			NSD	NSD	NSD
			R8	NR/NSD			R8	NSD	NSD				R8	XY+16			NSD	NSD	NSD
			R9	XY+16			R9	NSD	NSD				R9	XY+16			NSD	NSD	NSD
DI 1/16	XY+16	XY+16	R2	XY+16	XY+16	XY+16	R2	XY+16(A)@XY+16	XY+16	DI 1/16	XY+16	XY+16	R2	XY+16	XY+16	XY+16(A)@XY+16	XY+16	XY+16	XY+16
			R3	XY+16			R3	NSD	NSD				R3	XY+16			NSD	NSD	NSD
			R4	XY+16			R4	NSD	NSD				R4	XY+16			NSD	NSD	NSD
			R5	XY+16			R5	NSD	NSD				R5	XY+16			NSD	NSD	NSD

6.6 NucleoSpin® 8 Trace

The NucleoSpin® 8 Trace kit is designed for extraction of genomic DNA from forensic samples. Cell lysis is achieved by incubating samples in a solution containing chaotropic ions in the presence of proteinase K at room temperature. Adding isopropanol to the lysate creates the appropriate conditions for binding of DNA to the silica membrane, a process that is reversible and specific to nucleic acids. Inhibitors are removed by washing steps using an alcohol-containing buffer. Pure genomic DNA is eluted in a slightly alkaline elution buffer.

The evaluation of this kit was performed with slight alterations in the manual method to incorporate the use of the MultiPROBE® II PLUS PVM vacuum manifold, together with the

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

NucleoSpin® 8 Trace Starter Set A containing Column Holders A and Dummy Strips to enable use of the vacuum manifold.

The time to process a batch of 12 samples using the NucleoSpin® 8 Trace system takes about 5 hours, including a 3 hour incubation step. Each extraction batch included a positive and negative control, and also a substrate blank. Purified DNA was eluted in a final volume of 100µL.

Comparison of quantitation results for cell samples

Refer to Table 4 for observed data. NucleoSpin® 8 Trace produced greater mean concentration values and mean yields than the Chelex® protocol.

Comparison of quantitation results for blood samples

Refer to Table 5 for observed data. Mean blood quantitation values for samples extracted using NucleoSpin® 8 Trace were comparable to Chelex® results. Yields were variable but comparable to Chelex®.

Comparison of DNA profiles

NucleoSpin® 8 Trace overall yielded higher allele counts compared to Chelex®, resulting in 202 reportable alleles in contrast to the 89 alleles from Chelex®-extracted samples (Table 14). NucleoSpin® 8 Trace was able to yield profiles for cell samples on denim down to 1/8 dilution, but performed poorly with FTA® samples, resulting only in a partial profile (X,X+5) for the neat cell sample. NucleoSpin® 8 Trace performed better for cells on cotton swabs, and performed moderately better for cells on rayon swabs. Profiles from cells on cotton cloth samples were comparable between the two DNA extraction methods.

Table 14. Comparison of DNA profiles for cell substrate samples extracted using either Chelex® or NucleoSpin® 8 Trace.

CELLS Method: Chelex							CELLS Method: NucleoSpin 8 Trace						
Dilution	FTA		Cotton swabs		Rayon swabs		Dilution	FTA		Cotton swabs		Rayon swabs	
	Profile	Profile	Profile	Profile	Profile	Profile		Profile	Profile	Profile	Profile	Profile	Profile
Neat	XX+18	XX+18	R14	NSD	XX+8	NR/NSD	Neat	XX+6	XX+18	R14	AI/BD3	XX+18	XX+18
			R15	NR/NSD						R15	XX+18		
			R16	NSD						R16	XX+18		
			R17	NSD						R17	AI/BD3		
DI 1/4	XX+18	XX+18	R10	NSD	NR+1	NR/NSD	DI 1/4	NSD	XX+18	R10	XX+18	NR/NSD	XX+18
			R11	NSD						R11	XX+8		
			R12	NSD						R12	XX+1		
			R13	NSD						R13	NR/NSD		
DI 1/8	XX+17	XX+13	R6	NSD	XX+9	NR/NSD	DI 1/8	NSD	XX+17	R6	XX+17	NR/NSD	XX+13
			R7	NSD						R7	NR/NSD		
			R8	NSD						R8	XX+17		
			R9	NSD						R9	XX+17		
DI 1/16	NSD	NSD	R2	NSD	NSD	NSD	DI 1/16	NSD	NSD	R2	NSD	NSD	NSD
			R3	NSD						R3	NSD		
			R4	NSD						R4	NSD		
			R5	NSD						R5	NSD		
										R6	XX+17	NR/NSD	XX+13

For blood samples on rayon swabs, NucleoSpin® 8 Trace profiles were comparable to Chelex®, with several partial profiles being observed in the neat and 1/8 dilutions (Table 15).

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Table 15. Comparison of DNA profiles for blood substrate samples extracted using either Chelex® or NucleoSpin® 8 Trace.

BLOOD		Method: Chelex				Method: NucleoSpin 8 Trace			
Dilution	FTA	Cotton swabs	Rayon swabs		Cotton	Denim	Rayon swabs		
	Profile	Profile	Sample#	Profile	Profile	Profile	Sample#	Profile	
Neat	NSD	NSD	R14	X,Y+18	X,Y+18	NSD	R14	X,Y+18	Al@Am6L&D18
			R15	X,Y+18			R15	NR/NSD	
			R16	X,Y+18			R16	X,Y+18	
			R17	NR/NSD			R17	X,Y+18	
Dil 1/4	X,Y+18	X,Y+18	R10	Not Uploaded	X,Y+18	X,Y+18	R10	X,Y+18	
			R11	X,Y+18			R11	X,Y+18	
			R12	X,Y+18			R12	X,Y+18	
			R13	X,Y+18			R13	X,Y+18	
Dil 1/8	X,Y+18(Al@C)	X,Y+18	R6	X,Y+18	X,Y+18	X,Y+18	R6	X,Y+18	
			R7	X,Y+18			R7	X,Y+18	
			R8	NR/NSD			R8	X,Y+18	
			R9	X,Y+18			R9	X,Y+18	
Dil 1/16	X,Y+18	X,Y+18	R2	X,Y+18	X,Y+18	X,Y+18	R2	X,Y+18	
			R3	X,Y+18			R3	X,Y+18	
			R4	X,Y+18			R4	X,Y+18	
			R5	X,Y+18			R5	X,Y+18	

6.7 Summary

Findings from the evaluation of various forensic DNA extraction kits, compared to the in-house Chelex® protocol, is summarised in Table 16.

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND FORENSIC SERVICE

Table 16. Summary of findings from the evaluation of five forensic DNA extraction chemistries.

	Chelex	DNA IQ™	QIAamp® DNA Micro	ChargeSwitch®	forensic GEM™	NucleoSpin® 8 Trace
Processing time for 12 samples	2hr	3hr	5hr	1hr	2.5hr	5hr
Washing steps included to remove inhibitors	No	Yes	Yes	Yes	No	Yes
Final extract volume (µL)	~150	100	45	100	100 for FTA, 200 for other samples	100
% zero quantitation values for cells	43.750	9.375	37.500	0.000	9.375	24.140
% zero quantitation values for blood	0.000	0.000	0.000	0.000	0.000	0.000
Cell substrate displaying highest quant value for neat cell samples	FTA	Cotton swab	Cotton swab	Cotton swab	Cotton swab	Cotton cloth
Total number of reportable alleles for cells (max 576)	89	282	156	138	209	202
Total number of reportable alleles for blood (max 288)	234	252	264	288	25	264
Total number of autosomal loci exhibiting allelic imbalance (max 432)	1	1*	3	5	1	6^
Neat cell samples on denim showed inhibition (no profile)	Yes	No	Yes	Yes	No	No
Neat blood samples on rayon swabs showed inhibition (no profile)	No	No	No	No	Yes	No
Amenable to automation	No	Yes	Yes	Yes	Yes	Yes
Validated MultiPROBE II PLUS automated protocol	No	Yes	No	No	No	No

* Five occurrences of allelic imbalance were observed in Amelogenin.

^ One occurrence of allelic imbalance was observed in Amelogenin.

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Out of all the chemistries tested, only the Chelex® method and *forensicGEM*™ protocols do not incorporate washing steps for the removal of inhibitors and residual proteins. This is because in these protocols, the DNA is free in solution and not immobilised on to a capture device such as magnetic beads, and therefore washing of the sample cannot be performed. Washing steps result in high quality, purified DNA extracts. As such, Chelex® and *forensicGEM*™ extracts are considered to be crude DNA extracts of suboptimal quality that may not yield the best DNA profiles due to the presence of inhibitors that can affect PCR amplification of multiple STR loci. Although the dye in denim material did not appear to result in inhibition for *forensicGEM*™ samples, only 25/288 alleles (8.7%) from blood samples could be resolved by this extraction method.

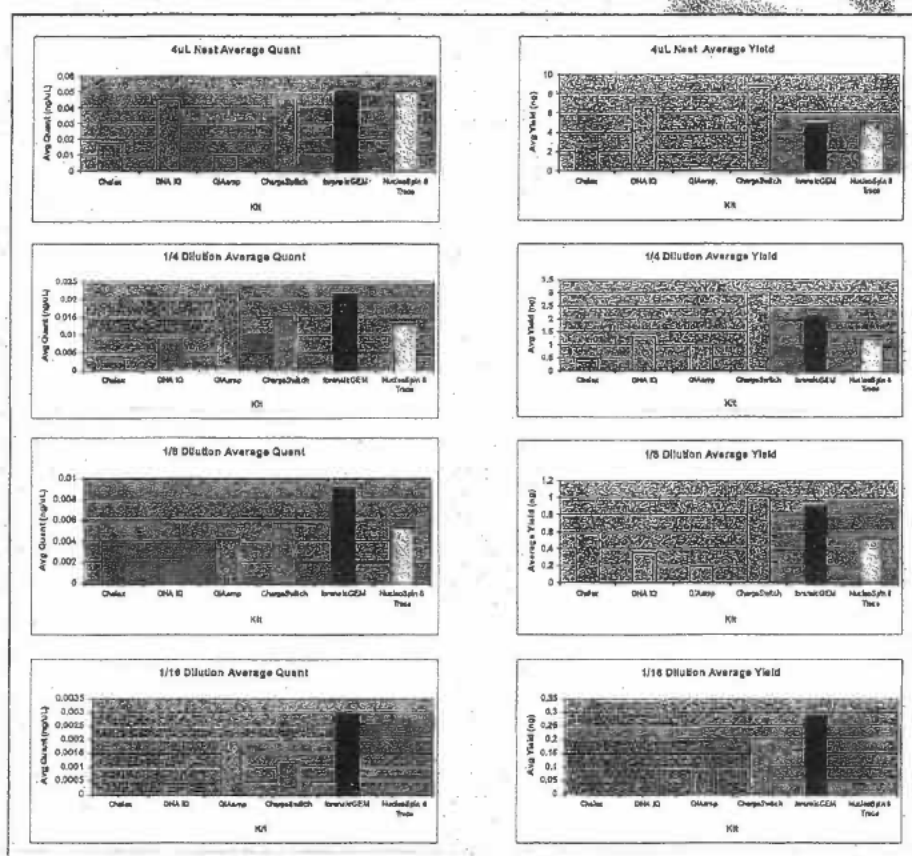


Figure 1. Average quantitation values (ng/μL) and yields (ng) for cell samples extracted using the various extraction chemistries tested, compared to Chelex®.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Although all kits resulted in quantitation results for all blood samples (0% had zero results), the results for cell samples exhibited more variation. Out of the extraction chemistries that incorporate washing steps, the DNA IQ™ system exhibited the best result for zero quantitation values for both cell and blood samples at 0% and 0% respectively. Almost half (44%) of Chelex® cell extracts failed to yield quantitation results. The next worst quantitation results were observed for QIAamp® DNA Micro (37.5% had zero results) followed by ChargeSwitch® (31.25%) and NucleoSpin® 8 Trace (24.14%). For all the different substrate types tested, average quantitation values were comparable for DNA IQ™, ChargeSwitch®, forensicGEM™ and NucleoSpin® 8 Trace in neat, 1/4 and 1/8 dilutions (Figure 1). Compared to samples extracted using Chelex®, samples extracted using the evaluated kits displayed higher average quantitation results that were up to 7.7 times higher than Chelex® results. Chelex® and NucleoSpin® 8 Trace were the only two kits that did not result in quantitation values for the 1/16 dilutions. The average yields varied widely due to different elution volumes for the various kits. For neat samples, DNA IQ™, ChargeSwitch®, forensicGEM™ and NucleoSpin® 8 Trace resulted in comparable yields for neat samples, which were on average double the yield generated by Chelex® (Figure 1). In all experiments, forensicGEM™ resulted in the highest quantitation values, but as discussed in the previous paragraph, this kit produced the least number of reportable alleles for blood samples. It was preferred to have a high quantitation result, coupled with a high yield and high final volume as it allows multiple tests to be performed.

The relationship between quantitation result and the number of resolved reportable alleles is close to proportional. A list of the evaluated chemistries, ranked according to the lowest to highest percentage of zero quantitation results, and also the most to the least number of resolved alleles, is outlined in Table 17.

Table 17. A ranking of the evaluated kits based on quantitation and DNA profile results.

Rank	% zero quantitation values	Total alleles for cells	Total alleles for blood
1	DNA IQ™ & forensicGEM™	DNA IQ™	ChargeSwitch®
2	NucleoSpin® 8 Trace	forensicGEM™	QIAamp® DNA Micro
3	ChargeSwitch®	NucleoSpin® 8 Trace	NucleoSpin® 8 Trace
4	QIAamp® DNA Micro	ChargeSwitch®	DNA IQ™
5	Chelex®	Chelex®	Chelex®
6		QIAamp® DNA Micro	forensicGEM™

The DNA IQ™ system was ranked the highest for most categories and performed the best for both cell and blood samples (see also Figures 2 and 3). For blood samples on rayon swabs, DNA IQ™ received a lower ranking due to 2 outlier results for neat dilutions as discussed above, but overall was considered to produce the best result for all dilutions. In contrast, Chelex® had the lowest rating as it was found to result in the least number of reportable alleles for both cell and blood samples. forensicGEM™ also outperformed the other kits for cell samples but performed very poorly for neat blood samples, indicating an inhibitory effect due to dissolved heme, although PCR amplification performance was improved in extracts of diluted blood samples (Figure 3). In contrast, QIAamp® DNA Micro worked well for blood samples, but performed the worst for cell samples. ChargeSwitch®, the alternative magnetic bead system to DNA IQ™, also performed better for blood samples than cell samples. The NucleoSpin® 8 Trace system, another membrane-based technology, performed moderately well and was ranked 3rd for the total number of alleles resolved for both cell and blood samples. Our results did not clearly indicate as to which technology, i.e. magnetic bead or silica membrane, was overall a better DNA extraction technology for forensic samples. However, DNA IQ™ worked the best in our hands as a complete "out-of-the-box" solution for extracting both cell and blood samples on various types of substrates.

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

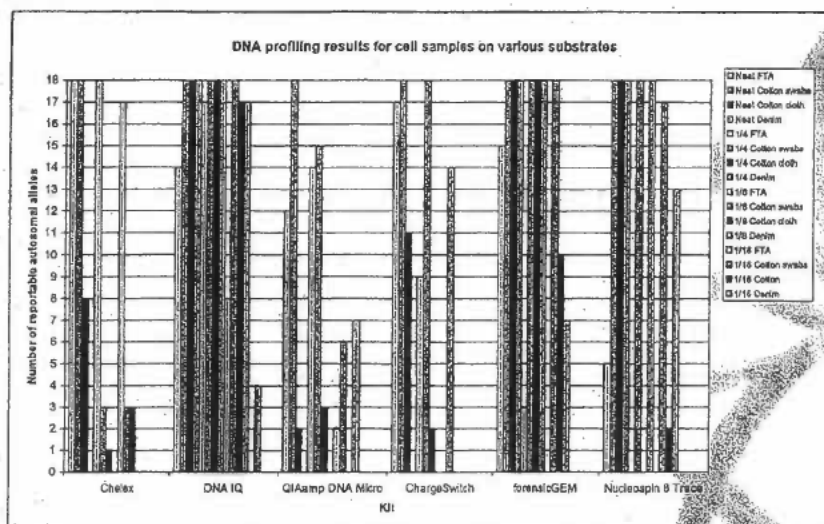


Figure 2. Total number of reportable alleles generated for cell samples on various substrates that were extracted using the various extraction chemistries tested, compared to Chelex[®]. The kit displaying the most number of full bars (i.e. most full profiles) was found to be DNA IQ[™], indicating the superior performance of this kit over the other kits tested. The current in-house Chelex[®] method did not perform as well as several of the tested kits.

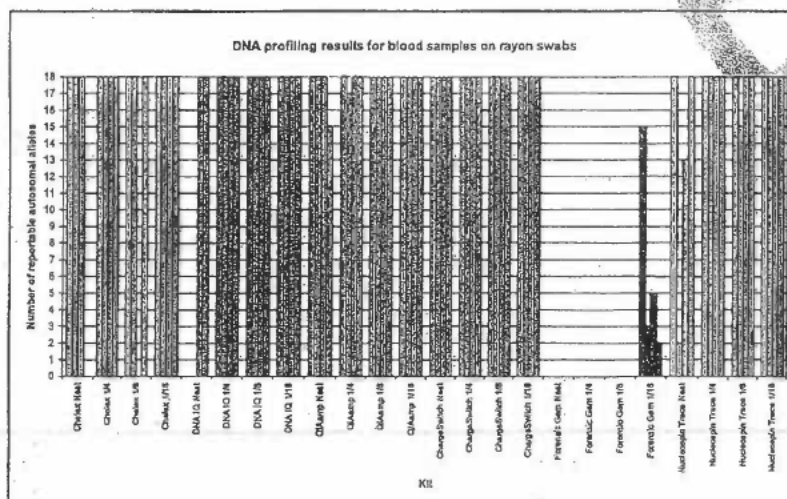


Figure 3. Total number of reportable alleles generated for blood samples on rayon swabs that were extracted using the various extraction chemistries tested, compared to Chelex[®]. All kits were able to resolve profiles from most dilutions, except forensicGEM[™] which could only resolve alleles from the 1/16 dilution, indicating an inhibitory effect of heme on the forensicGEM[™] system.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Out of a total of 432 loci amplified in the assessment of each kit, only one occurrence of allelic imbalance (AI; where peak height ratio is <70%) was detected in each of the Chelex[®], DNA IQ[™] and forensicGEM[™] kits (Table 16). QIAamp[®] DNA Micro and ChargeSwitch[®] each showed 3 and 5 occurrences of AI respectively, and NucleoSpin[®] 8 Trace showed the most AI at 6 occurrences observed (Table 16).

Out of 17 occurrences of AI in all samples tested, 9 AI events were observed in cell samples and 8 events were observed in blood samples (Table 18). These results do not suggest any increased likelihood in observing AI in either cell or blood samples. Out of the 9 AmpFISTR[®] Profiler Plus loci interrogated, AI was only encountered in 6 loci: D3S1358, FGA, D13S317, D8S1179, D18S51, and D7S820 (Table 18). Most of the AI (35.29%) occurred in the D13S317 locus, and the least (5.88%) occurred in both D8S1179 and D7S820. The %AI observed was within the range of 52.30% at D13S317 to 69.96% at D3S1358 (data not shown). Most of the AI (58.82%) was ≥60%, and 41.18% of AI was ≤65%. Out of the 7 occurrences of AI that were ≤60%, 4 events (57%) were observed in cell samples extracted using NucleoSpin[®] 8 Trace. Six additional occurrences of AI were observed in Amelogenin, with all AI events ≥60% (data not shown). The AI data from this evaluation will contribute to further studies on a revised in-house AI threshold.

Table 18. Frequency of all autosomal allelic imbalance observed in the evaluation

Kit	Number of autosomal AI		Profiler Plus loci exhibiting allelic imbalance					
	Cell	Blood	D3S1358	FGA	D13S317	D8S1179	D18S51	D7S820
Chelex	0	1	1					
DNA IQ	1				1			
QIAamp DNA Micro	1	2				1	2	
ChargeSwitch	2	3	1	1	2			1
forensicGEM		1			1			
NucleoSpin 8 Trace	5	1	2	1	2		1	
Total	9	8	4	2	6	1	3	1
		17	23.53%	11.76%	35.29%	5.88%	17.65%	5.88%

Neat cell or blood samples that were extracted using the various kits displayed varying inhibition results for denim dye and heme (Table 16). In several cases, if a kit did not show inhibition for denim dye, it would show inhibition for heme, or vice versa. Only the DNA IQ[™] and NucleoSpin[®] 8 Trace systems did not indicate inhibition for either inhibitor. There did not appear to be a link between the presence or absence of inhibition and the observation of allelic imbalance, although DNA IQ[™] and NucleoSpin[®] 8 Trace generated the most number of total reportable alleles (534 and 466 alleles respectively). These results suggest that the ability to remove inhibitors (such as encountered in the DNA IQ[™] and NucleoSpin[®] 8 Trace protocols) can result in an increase in the number of resolvable alleles, therefore successfully obtaining more DNA profile results more often.

Cotton substrates (e.g. cotton swabs and cotton cloth) make up a large percentage of samples processed in DNA Analysis FSS. For example, cotton swabs make up around 45% of the total number of sample types analysed for DNA analysis (Figure 4). It was therefore considered important that the DNA extraction kits evaluated could process samples and stains on cotton matrices. It was found that the neat cell samples that displayed the highest quantitation values across all extraction kits originated from cotton swab substrates, except for Chelex[®] results where the best result came from FTA (Table 16).

GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

All of the forensic DNA extraction kits evaluated are amenable to automation, and automated protocols already exist for several kits. However, only the DNA IQ™ kit has been validated for use on the MultiPROBE® II PLUS HT EX platform and a validated protocol was developed by PerkinElmer (PerkinElmer, 2004).

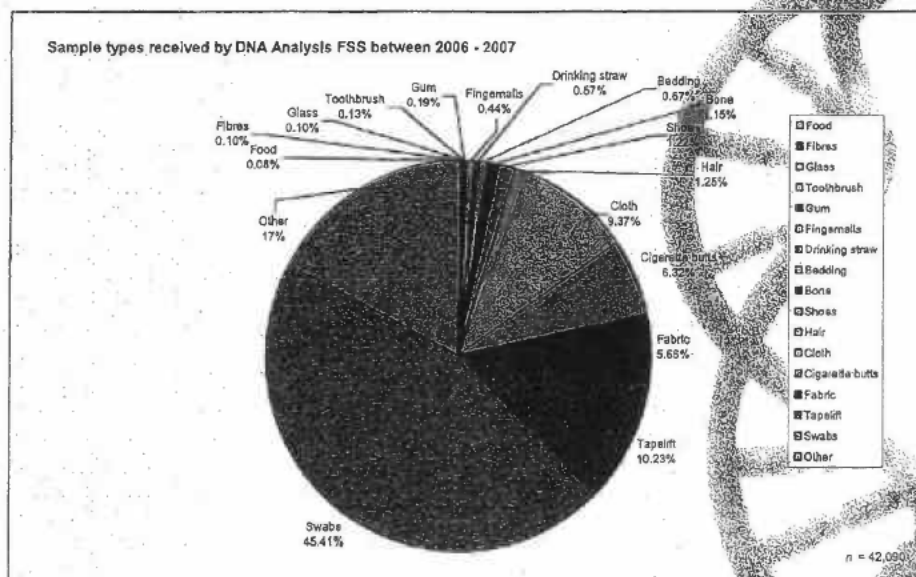


Figure 4. Pie chart of various sample types received by DNA Analysis FSS between 2006 and 2007. Around 45% of samples received for DNA analysis are swab substrates. Data was obtained from AUSLAB on 14 November 2007.

Some of the concerns raised regarding some of the kits tested include:

- QIAamp® DNA Micro involved multiple tube transfers that increased the risk of cross-contamination and also increased processing time to 5 hours for 12 samples.
- An increased risk of contamination was also prevalent in the NucleoSpin® 8 Trace method when coupled with the PVC vacuum manifold, because of the need to fit multiple adapters to ensure seals are maintained for a proper vacuum environment. If the plates and adapters were not assembled correctly, the vacuum environment would fail and possibly cause cross-contamination and, more alarmingly, loss of sample. Furthermore, even when assembled correctly, biohazardous contaminants (e.g. blood) are drawn down the manifold through the vacuum tubing and into the collection containers. Decontamination of the tubing and containers raises serious health and safety concerns.
- The forensicGEM™ system was the quickest protocol to perform and yielded crude DNA extracts that produced high allele counts for cell samples. However, the system could not deal with blood samples (and heme inhibition) effectively, therefore causing very low allele counts for blood samples.
- ChargeSwitch® was the alternative magnetic bead system to DNA IQ™. However, ChargeSwitch® did not produce results that were comparable or better than DNA

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

IQ™. For example, more ChargeSwitch® samples did not yield quantitation results compared to DNA IQ™ and resulted in a lower total allele count. ChargeSwitch® also did not appear to be able to effectively deal with inhibition from the dye in denim material.

Overall, data from the evaluation suggested that DNA IQ™ outperforms all of the forensic DNA extraction kits tested, in addition to the in-house Chelex® protocol. In summary, DNA IQ™:

- Is quick to perform – the amount of time taken to complete the DNA extraction protocol is comparable to the in-house Chelex® method;
- Includes washing steps to remove inhibitors – washing of the immobilised DNA enables purified DNA template to be eluted;
- Produced DNA quantitation values for most (>90%) samples – the percentage of samples that did not yield a quantitation result was one of the lowest for DNA IQ™;
- Generated the highest number of total reportable alleles – samples extracted using DNA IQ™ produced 65% more resolved alleles compared to Chelex®;
- Exhibited minimal allelic imbalance – the occurrence of AI in DNA IQ™ samples was comparable to Chelex®, although increased AI in Amelogenin was observed;
- Was not inhibited by heme in blood samples;
- Was not inhibited by the dye in denim material;
- Has been validated for use on the MultiPROBE® II PLUS HT EX platform.

7. Recommendations

Based on the results from evaluating various commercial DNA extraction kits that were designed specifically for forensic use, and comparing results from each kit to the current in-house Chelex® protocol, we have found DNA IQ™ to be the most suitable kit for extracting cell and blood samples that are analysed in DNA Analysis FSS. We therefore recommend that further studies be performed on the DNA IQ™ system in order to:

1. Validate a manual DNA IQ™ protocol for extracting various DNA Analysis FSS substrate types;
2. Verify an automated DNA IQ™ extraction program on the MultiPROBE® II PLUS HT EX platforms for automated DNA extraction of various DNA Analysis FSS substrate types.

8. References

- Butler J (2005). *Forensic DNA Typing*. Elsevier: Burlington, MA, USA.
- Gallagher B, Hlinka V, Muharam I, Iannuzzi C, Lundie G, Nurthen T, Ientile V (2007). Mock sample creation for cell and blood samples [Laboratory Report]. DNA Analysis FSS, Brisbane, QLD, Australia.
- Invitrogen Life Technologies (2005). ChargeSwitch® Forensic DNA Purification Kits for purification of genomic DNA from forensic samples [PN 25-0825, Version A, 3 January 2005]. Invitrogen Corporation: Carlsbad, CA, USA.
- Macherey-Nagel (2003). NucleoSpin® 8 Trace: Genomic DNA from Forensic Samples [Rev 0.2, November 2003]. Macherey-Nagel: Düren, Germany.
- Moss D, Harbinson S-A, Saul DJ (2003). An easily automated, closed-tube forensic DNA extraction procedure using thermostable proteinase. *Int J Legal Med* 117:340-349.
- PerkinElmer (2004). MultiPROBE II Liquid Handling Forensic Workstation Application Guide: Automated DNA IQ™ System for Mixed Casework Sample DNA Isolation [PN 8842157]. PerkinElmer Life and Analytical Sciences: Downers Grove, IL, USA.
- Promega Corporation (2006). DNA IQ™ System – Small Sample Casework Protocol [PN TB296, Rev. 4/06]. Promega Corporation: Madison, WI, USA.



Queensland Government
Queensland Health

GN-02

CaSS | Forensic and Scientific Services

A CRIMINAL AND STATEWIDE SERVICE

Qiagen (2003). QIAamp® DNA Micro Handbook [Rev. 08/2003]. Qiagen GmbH: Hilden, Germany.

QIS 19171 (2007). Method for Chelex® Extraction [Standard Operating Procedure]. DNA Analysis FSS: Brisbane, QLD, Australia.

Scott S, Harbison S-A, Saul DJ (2003). Developmental validation of *forensicGEM*™: a Thermophilic Proteinase for Forensic DNA Extraction [oral presentation at the 18th International Symposium on the Forensic Sciences, Fremantle, WA, 2-7 April 2006]. Institute of Environmental Research Ltd: Hamilton, New Zealand.

Walsh PS, Metzger DA, Higuchi R (1991). Chelex®-100 as a medium for simple extraction of DNA for PCR-based typing from forensic material. *Biotechniques* 10:506-13.

ZyGEM (2006). DNA extraction from buccal swabs using *forensicGEM*™. ZyGEM Corporation Ltd: Hamilton, New Zealand.


GN-02

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Copyright protects this publication. However, Queensland Health has no objection to this material being reproduced with acknowledgment, except for commercial purposes.

Permission to reproduce for commercial purposes should be sought from the QHSS DNA Analysis, 39 Kessels Rd, Coopers Plains 4108.
(07) 3274 9178

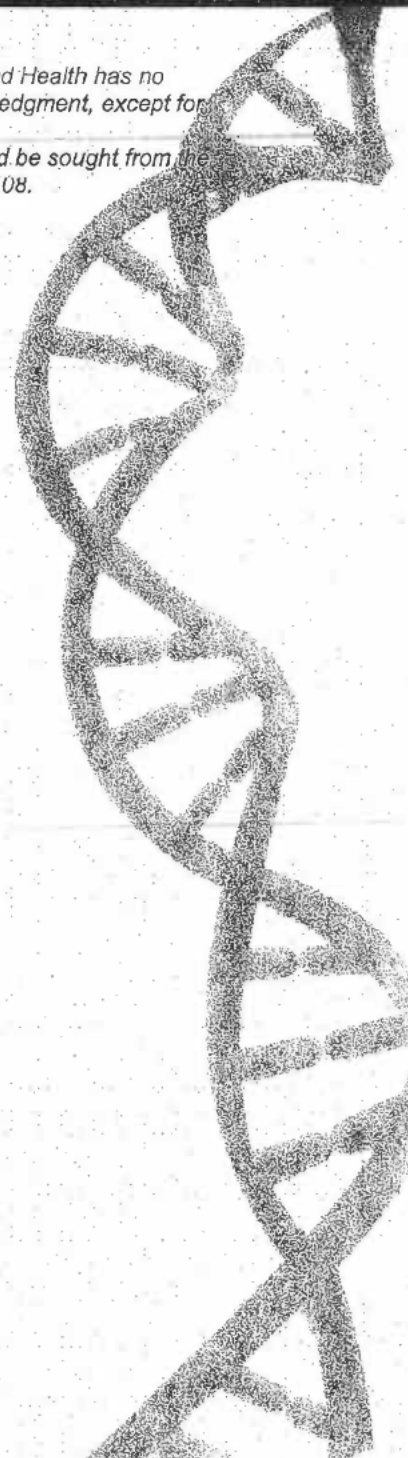

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Project 11. Report on the Validation of a manual method for Extracting DNA using the DNA IQ™ System

August 2008

Automation and LIMS Implementation Project Team,

DNA Analysis

Forensic And Scientific Services

Clinical and Scientific Services

Queensland Health

safe | sustainable | appropriate



Queensland Government
Queensland Health

CaSS | Forensic and Scientific Services

A CLINICAL AND STATISTICAL SERVICE

Project 11. Report on the Validation of a Manual Method for Extracting DNA using the DNA IQ™ System

Nurthen, T., Hlinka, V., Muharam, I., Gallagher, B., Lundie, G., Iannuzzi, C., Ientile, V.
Automation/LIMS Implementation Project, DNA Analysis FSS (August 2008)

1. Abstract

The DNA IQ™ system was found to be the most suitable kit for extracting cell and blood samples that are analysed in DNA Analysis FSS (refer to Project 9). This DNA extraction system, based on magnetic bead technology, was found to generate results that were comparable or better than the current Chelex®-100 protocol. We have validated a manual DNA IQ™ method for extracting DNA from forensic samples, and incorporated studies on sensitivity and consistency, inhibition, substrate type, substrate size, and mixture studies. This manual DNA IQ™ method is suitable for verification on the automated MultiPROBE® II PLUS HT EX extraction platforms.

2. Introduction

A previous evaluation of various DNA extraction systems that were designed specifically for forensic samples was performed in order to select a suitable extraction technology for extracting various sample types that are processed in DNA Analysis FSS. DNA IQ™ was identified as a suitable kit for extracting forensic samples, and was found to outperform both the current Chelex®-100 protocol and also all the other kits evaluated. The results of the evaluation are reported in Project 9 (Gallagher *et al.*, 2007a).

DNA purification with silica matrices, either in membrane- or bead-form, commonly uses the affinity of DNA for silica without the need for hazardous organic reagents. However, these systems tend to require extensive washing to remove the guanidium-based lysis buffer. The DNA IQ™ system uses a novel paramagnetic resin for DNA isolation (Promega Corp., 2006). The DNA IQ™ System's basic chemistry is similar to other silica-based DNA isolation technologies, except that the specific nature of the paramagnetic resin, coupled with the formulation of the lysis buffer, is unique. In the DNA IQ™ System, negatively-charged DNA molecules have a high affinity for the positively-charged paramagnetic resin under high salt conditions supplied by the lysis buffer. Once DNA is bound to the magnetic resin, and the resin is immobilised by a magnet, the sample can be washed using an alcohol/aqueous buffer mixture. The high alcohol content of the wash buffer aids to maintain the DNA-resin complex in low-salt conditions, while the aqueous component functions to wash away residual lysis buffer and any inhibitors or non-DNA contaminants such as cellular debris and protein residues. DNA is released from the resin by using a low ionic strength elution buffer, and the purified DNA can be used directly in downstream applications such as PCR.

For samples that are in excess (e.g. reference samples), DNA IQ™ resin will only isolate up to a total of approximately 100ng of DNA due to bead saturation (Huston, 2002).

3. Aim

To validate a manual method for DNA extraction of blood and cell stains on forensic samples using the DNA IQ™ system (Promega Corp., Madison, WI, USA).

CaSS | Forensic and Scientific Services

A CLINICAL AND STATISTICAL SERVICE

4. Equipment and Materials

- DNA IQ™ System (Promega Corp., Madison, WI, USA); 100 samples, Cat.# DC6701), which includes:
 - 0.9mL Resin
 - 40mL Lysis Buffer
 - 30mL 2X Wash Buffer
 - 15mL Elution Buffer
- TNE buffer (10mM Tris, 100mM NaCl, 1mM EDTA, pH 8.0)
- MagneSphere® Magnetic Separation Stand, 12-position (Cat.# Z5342) (Promega Corp., Madison, WI, USA)
- DNA IQ™ Spin Baskets (Cat.# V1221) (Promega Corp., Madison, WI, USA)
- Microtube 1.5mL (Cat.# V1231) (Promega Corp., Madison, WI, USA)
- 95-100% ethanol
- Isopropyl alcohol
- 1M DTT (Sigma-Aldrich, St. Louis, MO, USA)
- Proteinase K (20mg/mL) (Sigma-Aldrich, St. Louis, MO, USA)
- 20% SDS (Biorad, Hercules, CA, USA)
- 0.9% saline solution (Baxter Healthcare, Old Toongabbie, NSW, Australia)
- ThermoMixer Comfort (Eppendorf, Hamburg, Germany)
- Vortex mixer
- Bench top centrifuge
- Cytobrush® Plus Cell Collector (Cooper Surgical, Inc., Trumbull, CT, USA)
- FTA® Classic Cards (Whatman plc, Maidstone, Kent, UK)
- Rayon (155C) and cotton (164C) plain dry swabs (Copan Italia S.p.A., Brescia, Italy)
- Vacuette® K2EDTA blood collection tubes (Greiner Bio-One GmbH, Frickenhausen, Germany)
- Sticky tape (BDF tesa tape Australia Pty Ltd)
- Tannic acid $C_{76}H_{52}O_{48}$ FW1701.25 (Selby's BDH, Lab Reagent >~90%)
- Urea NH_2CONH_2 FW60.06 (BDH, Molecular Biology Grade ~99.5%)
- Indigo carmine $C_{16}H_8N_2Na_2O_8S_2$ FW466.35 PN 131164-100G (Sigma-Aldrich, St. Louis, MO, USA)
- Humic acid sodium salt PN H167520-100G (Sigma-Aldrich, St. Louis, MO, USA)
- Used car motor oil, SW20/SAE50 (Caltex)
- Various clothing materials, including:
 - Best & Less Pacific Cliff, White cotton shirt, XXL
 - Big W Classic Denim, Men's Blue denim jeans, 112
 - Private Encounters, off-white nylon cami, size 14
 - Clan Laird, blue 100% wool kilt
 - Millers Essentials, blue 100% polyester camisole, size 10
 - Unknown, teal green 100% lycra swimwear
 - Leather Belt, brown

5. Methods

5.1 Cell and blood collection

Buccal cells were collected using a modified Cytobrush® protocol (Mulot *et al.*, 2005; Satia-Abouta *et al.*, 2002). Four donors were chosen. Each donor was asked to brush the inside of one cheek for one minute. Then, with another Cytobrush®, the other cheek was also sampled. The cells collected on the brush were then resuspended in 2mL of 0.9% saline solution. Multiple collections were taken on different days.

CaSS | Forensic and Scientific Services

A CENTRAL AND STATEWIDE SERVICE

Whole blood was collected from three donors by a phlebotomist as per standard collection procedures in EDTA tubes. Blood samples were refrigerated until spotting onto substrate and cell-counting step.

Table 1 lists the donor sample ID's.

Table 1. List of donor samples used for validating a manual DNA IQ™ method.

Donor ID
<i>Cell samples</i>
D1
D2
D3
D4
<i>Blood samples</i>
D1
D2
D3

5.2 Cell counting

Buccal cell suspensions were diluted using 0.9% saline solution to create a 1/10 dilution of the original sample prior to submitting for cell counting. All counts were performed by the Cytology Department, RBWH (QIS 15393).

Blood cell counting was performed on a 1mL aliquot of the original sample also by the Cytology Department, RBWH (QIS 15393).

5.3 Sensitivity, Reproducibility (Linearity) and Yield

Sensitivity and reproducibility of the DNA IQ™ kit was assessed using dilutions of cell and blood samples.

For cell samples, dilutions were made using a sample from donor 4, diluted in 0.9% saline solution. The dilutions used were:

- Neat
- $1/10$
- $1/100$
- $1/1000$

For blood samples, dilutions were made using a sample from donor 2, diluted in 0.9% saline solution. The dilutions used were:

- Neat
- $1/10$
- $1/100$
- $1/1000$

Mock samples were created from rayon and cotton swabs using the above dilutions. The swab heads were removed from the shaft using sterilised scalpel and tweezers. Swab heads were then cut into quarters and each quarter was then added to separate sterile 1.5mL tubes. To each quarter swab, 30µL of each neat sample or dilution was added to

CaSS | Forensic and Scientific Services

A CITYWIDE AND STATEWIDE SERVICE

create a total of five replicates. Samples were dried using a ThermoMixer set at 56°C over 2 hours in a Class II biohazard cabinet.

5.4 Inhibition challenge

Quartered cotton swabs in sterile 1.5mL tubes were spotted with 30µL of neat cell suspension and were dried after each addition on a ThermoMixer as described previously. Neat blood samples were also created using the same method.

All the inhibitors except for the motor oil were obtained in powder form. Before making any liquid solution of the powdered inhibitors, research was conducted to determine the likely level of each inhibitor normally encountered in the environment (Hlinka *et al.*, 2007). Each solution was made at concentrations based on the information obtained (Table 2).

Table 2. Concentrations of various inhibitors used in the inhibition study.

Inhibitor	Excess/Neat Solution	Mass	Volume H ₂ O	Final inhibitor concentration
Tannic acid	Excess	600mg	500µL	0.705M
	Neat	200mg	500µL	0.235M
Humic acid	Excess	1g	5mL	20% (w/v)
	Neat	0.1g	5mL	2% (w/v)
Indigo carmine	Excess	0.47g	10mL	100mM
	Neat	0.047g	10mL	10mM
Urea	Excess	0.06g	1mL	1M
	Neat	0.021g	1mL	0.33M

A total of 30µL of each solution containing specified concentrations of various inhibitors was applied to the buccal cell and blood swabs prepared above. The only exception was motor oil, where only 15µL was added to the cell and blood swabs respectively. Each inhibitor sample was replicated in quadruplicate and left to dry overnight in a Class II biohazard cabinet.

To another set of prepared cell and blood swabs, an excess of each inhibitor was applied in quadruplicate for each inhibitor and allowed to dry overnight. This process was achieved by applying another solution of inhibitor exceeding the normal level (Hlinka *et al.*, 2007).

5.5 Substrates

Swabs

Four cotton and four rayon swab quarters in sterile 1.5mL tubes were loaded with 30µL of neat cell or blood sample and were extracted once the sample had dried on the swab.

Tapelifts

Two donors were sampled using the tape most commonly used within the laboratory (BDF tesa tape). Strips of tape were firmly applied to the inside of the fore arm and lifted off. This process was then repeated until the tape was no longer adhesive. The tape was wrapped around sticky-side-in, forming a cylinder shape, and placed in a sterile 1.5mL tube. These samples were created in quadruplicate. Tape was not used as a substrate in the blood validation.

Fabric

The material types tested included:

- Denim jeans;

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND WATOWIDE SERVICE

- White 100% cotton shirt;
- Blue 100% wool kilt;
- Teal green 100% lycra swimwear;
- White 100% nylon camisole;
- Blue 100% polyester camisole; and
- Brown 100% woven leather belt.

All material types except leather were sampled and ten 2.5cm x 2.5cm pieces were cut from each material and washed in 10% bleach following an in-house washing method to remove any contaminating DNA from outside the laboratory (Gallagher *et al.*, 2007b). As for the leather, one strand of the leather weave was cut from the belt and washed following the same method. Once dry, the material was then cut into 0.5cm x 0.5cm pieces using sterile techniques, placed in 1.5mL tubes and 30µL of both cell sample and blood was applied to separate pieces. Each substrate sample was created in quadruplicate and dried on a ThermoMixer set at 56°C over 2 hours in a Class II biohazard cabinet.

Gum

Two types of chewing gum were chosen: (1) Wriggley's Extra White (peppermint flavour) and (2) Wriggley's Extra Green (spearmint flavour). The donor was asked to chew the gum for 30 minutes and dispose of the gum into a clip-seal plastic bag. The gum was then air dried in a Falcon tube overnight before it was frozen for roughly an hour before cutting into 3mm x 3mm x 3mm pieces and placed into sterile 1.5mL tubes. Gum substrates were not assessed for blood samples.

Cigarette butts

Two brands of cigarettes were smoked all the way through and then the butts collected. The filter paper of the butt was cut into 0.5mm² pieces and placed into sterile 1.5mL tubes. Cigarette butts were not assessed for blood samples.

FTA® Classic Card punches

Eight sterile 1.5mL tubes, each containing four 3.2mm FTA® Classic Card punches, were spotted with 30µL of cells or blood before being dried on a ThermoMixer. Four replicates contained sample from one donor, the other remaining four replicate tubes had a different donor sample added.

5.6 Mixture studies

Buccal cells and whole blood were obtained from a male and female donor. Dilutions were made using 0.9% saline solution to ensure that the cell concentration was equal. Dilutions were then performed on the male sample to obtain the correct ratios.

Mock samples were created using the following ratios of female to male:

- 1:1,
- 1:2,
- 1:10,
- 1:25,
- 1:50 and
- 1:100.

A total of 30µL of the female component was spotted first on to a quarter of a cotton swab in a sterile 1.5mL tube and dried on a ThermoMixer before adding another 30µL of the male component. Samples were created in quadruplicate for all ratios, for both cell and blood samples.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

5.7 Substrate size

Various sizes of material were cut from a white cotton shirt:

- 0.5cm x 0.5cm,
- 1cm x 1cm,
- 2cm x 2cm.

Each piece of material was stored in individual, sterile 1.5mL tubes and 30µL of cell sample was added to the material and allowed to dry on a ThermoMixer. The same process was followed for blood samples. Five replicates were made for each sample type.

5.8 Extraction using the DNA IQ™ System (Promega Corp.)

The manual DNA IQ™ method used was based on an automated protocol developed by the Centre of Forensic Sciences (CFS) in Toronto, Ontario (PerkinElmer, 2004). A Proteinase K – SDS Extraction Buffer was made as per the recommended protocol.

The 1x Extraction Buffer for one sample consisted of:

277.5µL TNE buffer
15µL Proteinase K (20mg/mL)
7.5µL 20% SDS

The TNE buffer consisted of:

1.211g Tris (10mM Tris)
2mL 0.5M EDTA (1mM EDTA)
5.844g NaCl (100mM NaCl)

The adapted manual DNA IQ™ protocol is described below:

1. Set one ThermoMixer at 37°C and another at 65°C.
2. Ensure that appropriately sized samples are contained in a sterile 1.5mL tube. For every sample, prepare three set of labelled tubes: spin baskets (for every tube except the extraction control), 2mL SSI tubes and Nunc™ tubes.
3. Prepare Extraction Buffer and add 300µL to each tube. Close the lid and vortex before incubating the tubes at 37°C on the ThermoMixer at 1000rpm for 45 minutes.
4. Remove the tubes from the ThermoMixer and transfer the substrate to a DNA IQ™ Spin Basket seated in a labelled 1.5mL Microtube using autoclaved twirling sticks. Then transfer the liquid to a labelled 2mL SSI sterile screw cap tube.
5. Centrifuge the spin basket on a benchtop centrifuge at room temperature for 2 minutes at its maximum speed. Once completed, remove the spin basket and collect the remaining solution and pool with the original extract in the 2mL SSI sterile screw cap tube, then vortex.
6. Add 550 µL of Lysis Buffer to each tube.

GN-03

CaSS | Forensic and Scientific Services

7. Dispense 50µL of DNA IQ™ Resin – Lysis Buffer solution (7µL Resin in 43µL Lysis Buffer) to each tube. Invert the resin tube regularly to keep the beads suspended while dispensing to obtain uniform results.
 8. Vortex each tube for 3 seconds at high speed then place in a multitube shaker set at 1200rpm to incubate at room temperature for 5 minutes.
 9. Vortex each tube for 2 seconds at high speed before placing the tubes in the magnetic stand. Separation will occur instantly.
- Note:** If resin does not form a distinct pellet on the side of the tube, or if the pellet has accidentally mixed with the solution while in the stand, vortex the tube and quickly place back in the stand.
10. Carefully remove and discard all of the solution without disturbing the resin pellet on the side of the tube. If some resin is drawn up in tip, gently expel resin back into tube to allow re-separation.
 11. Remove the tube from the magnetic stand; add 125µL of prepared Lysis Buffer and vortex for 2 seconds at high speed.
 12. Return tube to the magnetic stand, allow for separation and then remove and discard the Lysis Buffer.
 13. Remove tube from the magnetic stand; add 100µL of prepared 1X Wash Buffer and vortex for 2 seconds at high speed.
 14. Return tube to the magnetic stand, allow for separation and then remove and discard all Wash Buffer.
 15. Repeat Steps 13 to 14 two more times for a total of three washes. Be sure that all of the solution has been removed after the last wash.
 16. In a biohazard cabinet, place the lids of the tubes upside down on a Kimwipe, in their respective order, and the tubes into a plastic rack, and air-dry the resin for 5-15 minutes at room temperature. Do not dry for more than 20 minutes, as this may inhibit removal of DNA. Once dry, screw on the lids.
 17. To each samples then add 50µL of Elution Buffer very gently on the top of the magnetic pellet. Do not mix.
 18. Close the lid and then incubate the tubes in the ThermoMixer at 65°C for 3 minutes with no shaking and another 3 minutes shaking at 1100 rpm.
 19. Remove the tubes and vortex for 2 seconds at high speed. Immediately place the tube in the magnetic stand. Tubes must remain hot until placed in the magnetic stand or yield will decrease.
 20. Carefully transfer the supernatant containing the DNA to the respective labelled Nunc™ tubes.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

21. Repeat step 17 to 20, transferring the supernatant to the appropriate Nunc™ tube. The final volume after the second elution should be approximately 95µL.

Note: DNA can be stored at 4°C for short-term storage or at -20 or -70°C for long-term storage.

5.9 DNA quantitation

All DNA extracts were quantified using the Quantifiler™ Human DNA Quantitation kit (Applied Biosystems, Foster City, CA, USA) as per QIS 19977. Reaction setup was performed on the MultiPROBE® II PLUS HT EX (PerkinElmer) pre-PCR platform.

5.10 PCR amplification

DNA extracts were amplified using the AmpFtSTR® Profiler Plus® kit (Applied Biosystems, Foster City, CA, USA) as per QIS 19976. Reaction setup was performed on the MultiPROBE® II PLUS HT EX (PerkinElmer) pre-PCR platform.

5.11 Capillary electrophoresis and fragment analysis

PCR product was prepared for capillary electrophoresis using the manual 9+1 protocol (refer to Project 15 and QIS 19978). Capillary electrophoresis was performed on an ABI Prism® 3100 Genetic Analyzer (Applied Biosystems, Foster City, CA, USA) under the following conditions: 3kV injection voltage, 10 sec injection time, 15kV run voltage, 100µA run current, and 45min run time. Data Collection Software version 1.1 was used to collect raw data from the ABI Prism® 3100 Genetic Analyzer. Fragment size analysis was performed using GeneScan 3.7.1. Allele designation was performed using Genotyper 3.7, with thresholds for heterozygous and homozygous peaks at 150 and 300 RFU respectively. The allelic imbalance threshold is 70%.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

6. Results and Discussion

6.1 Donor sample cell counts

Aliquots of buccal cell samples were counted at Cytology Department (RBWH) to determine the concentration of viable cells, in order to better estimate the number of cells at any particular dilution. A white cell count was not performed on all the blood samples, and therefore an estimate on the number of nucleated cells could not be determined.

6.2 Sensitivity, consistency and yield

To ensure the reliability and integrity of results for samples containing small amounts of DNA, a sensitivity study was conducted to determine the lowest concentration of DNA that provides reliable results. A consistency study was combined into the sensitivity experiment to determine the maximum acceptable difference between the results obtained. All samples were extracted in identical conditions by the same operator at the same time to minimise variability.

The cell sample used for the experiments was from donor sample 4A, which was counted to be around 3,680 nucleated cells ($\times 10^6/L$). The blood sample used was from donor 6A, which was counted to be around 2,540 nucleated cells ($\times 10^6/L$). The estimated amount of DNA present in each dilution is outlined in Table 3.

Table 3. Amount of DNA in each dilution, as calculated from the cell count.

Sample type	Dilution factor	Number of cells ($/\mu L$)	gDNA (ng/ μL)	Theoretical total DNA on swab (ng)
Cells	Neat	3680	23.552	706.56000
	1/10	368	2.3552	70.65600
	1/100	36.8	0.23552	7.06560
	1/1000	3.68	0.023552	0.70656
Blood	Neat	2540	16.256	487.68000
	1/10	254	1.6256	48.76800
	1/100	25.4	0.16256	4.87680
	1/1000	2.54	0.016256	0.48768

The DNA yields resulted from extracting the above cell dilutions using the DNA IQ™ System is outlined in Table 4. Blood samples produced higher yields compared to cell samples. On average, blood samples on cotton swabs generated the highest yields. Cell samples on rayon and cotton swabs generated similar yields. All blood dilutions down to 1/1000 produced quantitation results, but cell samples only produced reliable quantitation results down to 1/100 dilution, possibly due to the effects of cell clumping.

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Table 4. DNA quantitation data for diluted cell and blood samples on rayon and cotton substrates.

Sample type	Dilution factor	Theoretical Input DNA (ng)	Rayon swab yield (ng)	Alleles	Cotton swab yield (ng)	Alleles	Rayon average yield (ng)	Rayon Std Dev	Recovery Rayon (%)	Cotton average yield (ng)	Cotton Std Dev	Recovery Cotton (%)
Cells	Neat	706.56000	110.0000	18	117.0000	18	134.5400	41.30	19.04	95.2800	32.69	13.48
			130.0000	18	124.0000	18						
			160.0000	18	46.8000	18						
			83.7000	7	76.6000	18						
			189.0000	17	112.0000	18						
	1/10	70.65600	10.1000	18	12.8000	18	10.4520	1.44	14.79	10.4820	2.52	14.84
			12.7000	18	6.3100	18						
			9.5500	18	11.5000	18						
			9.0100	18	10.1000	18						
			10.9000	18	11.7000	18						
	1/100	7.06560	0.6350	0	0.0000	0	0.9254	0.64	13.10	0.1270	0.18	1.80
			0.4930	0	0.0000	0						
			1.4000	5	0.2770	0						
			1.7900	14	0.3580	0						
			0.3090	0	0.0000	0						
	1/1000	0.7656	0.0000	0	0.3630	0	0.0166	0.04	2.17	0.0726	0.16	9.48
			0.0000	0	0.0000	0						
			0.0000	0	0.0000	0						
			0.0000	0	0.0000	0						
			0.0831	0	0.0000	0						
Blood	Neat	487.68000	216.0000	18	718.0000	18	317.0000	102.36	55.00	447.0000	196.46	91.66
			447.0000	18	297.0000	18						
			215.0000	18	595.0000	18						
			383.0000	7	326.0000	18						
			324.0000	18	299.0000	18						
	1/10	48.76800	113.0000	18	126.0000	18	124.7800	28.10	255.86	97.6600	21.66	200.25
			107.0000	18	91.9000	18						
			145.0000	18	75.4000	18						
			95.9000	18	81.0000	18						
			163.0000	18	114.0000	18						
	1/100	4.87680	14.3000	18	15.9000	18	12.4800	1.62	255.91	16.7600	4.69	343.67
			12.5000	13	12.1000	18						
			13.2000	18	20.8000	18						
			9.9000	18	22.4000	18						
			12.5000	18	12.6000	18						
	1/1000	0.48768	0.7300	18	2.3700	18	0.8894	0.20	182.37	3.0200	0.85	619.26
			0.6990	18	3.1300	18						
			1.1800	18	3.6300	18						
			0.8670	18	1.9700	18						
			0.9710	18	4.0000	18						

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

The average yield observed within cell and blood samples on either rayon or cotton swabs were comparable (Figure 1). Some inconsistencies were present in cell samples at the lower dilutions of 1/100 and 1/1000 due to unreliable quantitation data at these low dilutions. Blood samples were found to generate higher average yields than cell samples and gave unexpectedly higher recovery values, despite the fact that the input DNA amount was 2-fold higher for cells compared to blood samples (Table 4). This discrepancy may have arisen from inconsistencies in cell suspension uniformity during dilutions of the original cell or blood sample, resulting in inaccurate estimates for average cell concentrations.

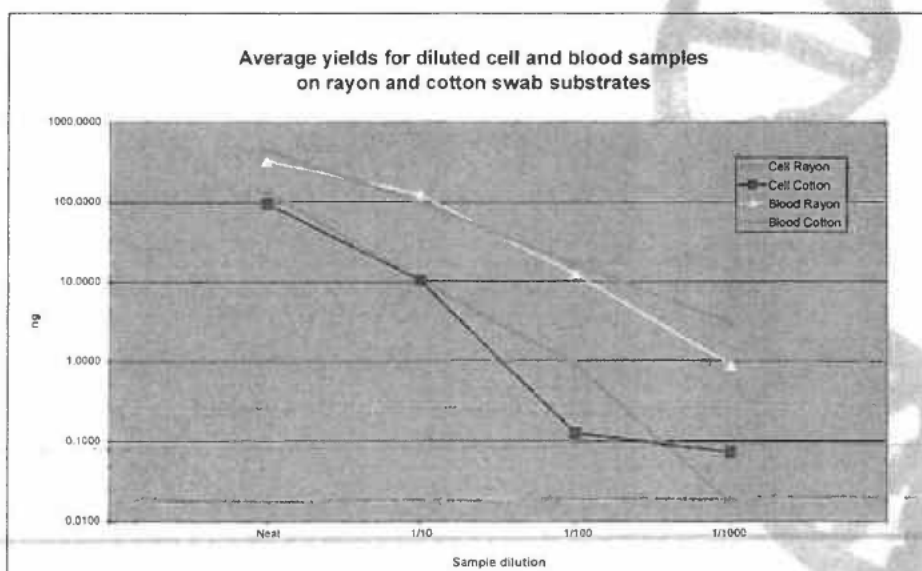


Figure 1. Average yields as observed in the sensitivity study. The yields for cell and blood samples, on two different swab types, were comparable as indicated by overlapping lines on the graph.

The dilution factor was, however, accurately reflected in the average yield for the various dilutions as displayed in Table 4 and Figure 2. An exception to this was the average yields for the neat dilutions (Figure 2). DNA IQ™ isolates a maximum of 100ng DNA as the resin is present in excess, and the system becomes more efficient with samples containing less than 50ng of DNA. Because the amount of DNA was in excess in neat samples, the observed yields varied from sample-to-sample. According to the manufacturer, the DNA IQ™ Database Protocol should be used for samples containing more than 100ng DNA to result in more consistent concentrations between the samples (Huston, 2002).

All five replicates for each neat dilution displayed the highest yields for each dilution series, as expected (Figure 2). For blood samples on rayon and cotton swabs, yields were still around 1ng for samples at the 1/1000 dilution (Figure 3).

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

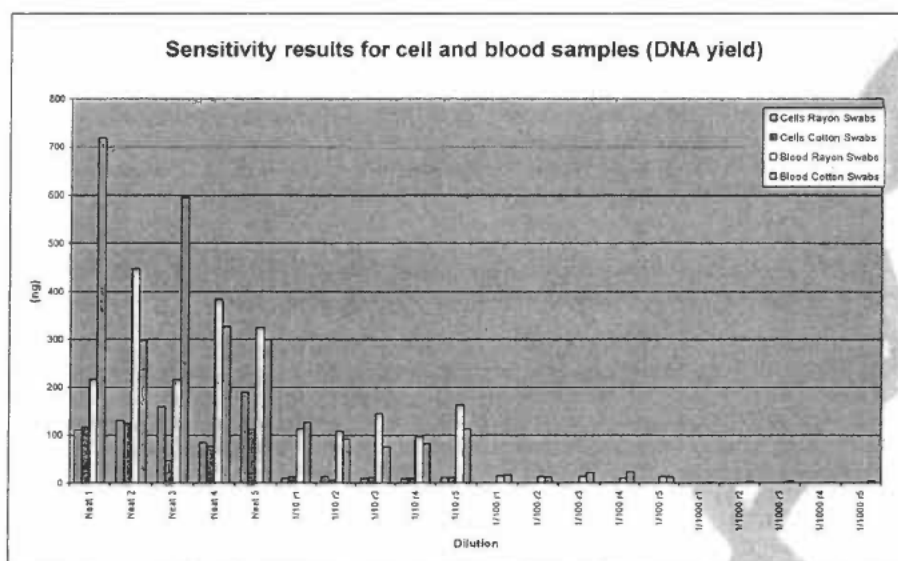


Figure 2. DNA yields (ng) observed for the sensitivity study. As expected, neat samples provided the highest yields. Yields were obtained down to 1/1000 for blood samples and 1/100 for cell samples.

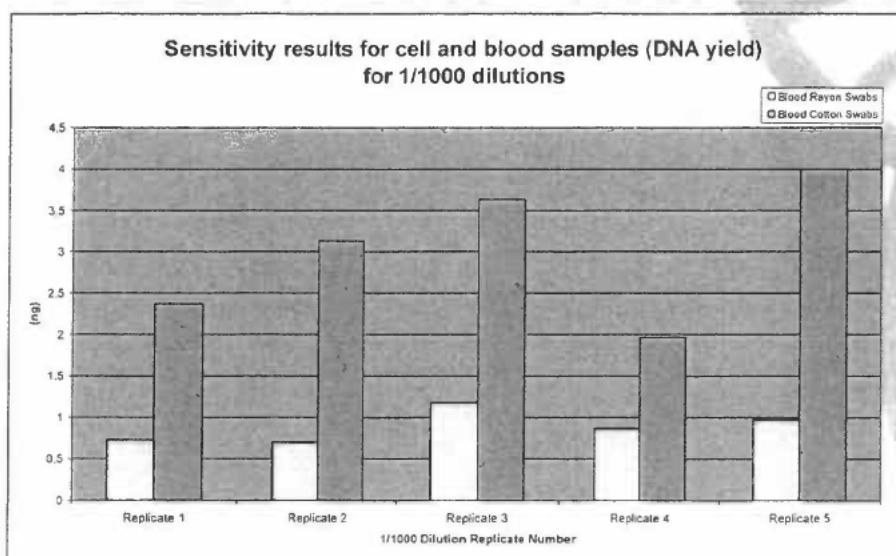


Figure 3. DNA yields (ng) observed for the sensitivity study, at the 1/1000 dilution.

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

When amplified using a 9-locus STR system, all neat samples produced the expected full DNA profile (18/18 alleles), although one outlier was encountered for a cell rayon sample which produced a 7/18 partial profile (Table 4). For cell samples, full profiles could be obtained for samples that were diluted down to 1/10, with partial profiles generated from samples diluted to 1/100. For blood samples, full profiles were generally obtained from all dilutions down to 1/1000. Although two partial profiles were encountered in blood samples on rayon swabs, all blood cotton swabs produced full profiles at all dilutions.

The apparent discrepancy between the results for cell and blood samples can be attributed to inaccurate cell counts or non-uniform sample suspensions when creating the dilutions, as caused by cell clumping or cellular breakdown and precipitation.

For five replicates of each dilution, consistency was observed to vary depending on the dilution (Figure 4). Consistency, as an indication of reproducibility, was calculated as the percentage of the yield standard deviation over five replicates divided by the mean yield of all five replicates ($\%[SD_{\text{yield}} / \text{mean}_{\text{yield}}]$). A value closer to 0% indicates minimal sample-to-sample variation and therefore the results are highly consistent. The mean combined reproducibility for all neat, 1/10, 1/100 and 1/1000 dilutions were 35.31%, 20.63%, 62.14% and 124.32% respectively (Figure 4), indicating that there was high reproducibility between the neat and 1/10 dilutions across the four sample types, and reduced reproducibility at the lower 1/100 and 1/1000 dilutions. Overall, the blood samples on rayon and cotton both exhibited high reproducibility across all dilutions at an average of 30.54% and 22.45% respectively (Figure 5). The cell rayon and cotton samples were more variable across all dilutions, producing lower reproducibility at an average of 84.23% and 105.19% respectively (Figure 5). The poor performance of the cell samples can be attributed to inconsistencies in quantitation data observed at the lower 1/100 and 1/1000 dilutions.

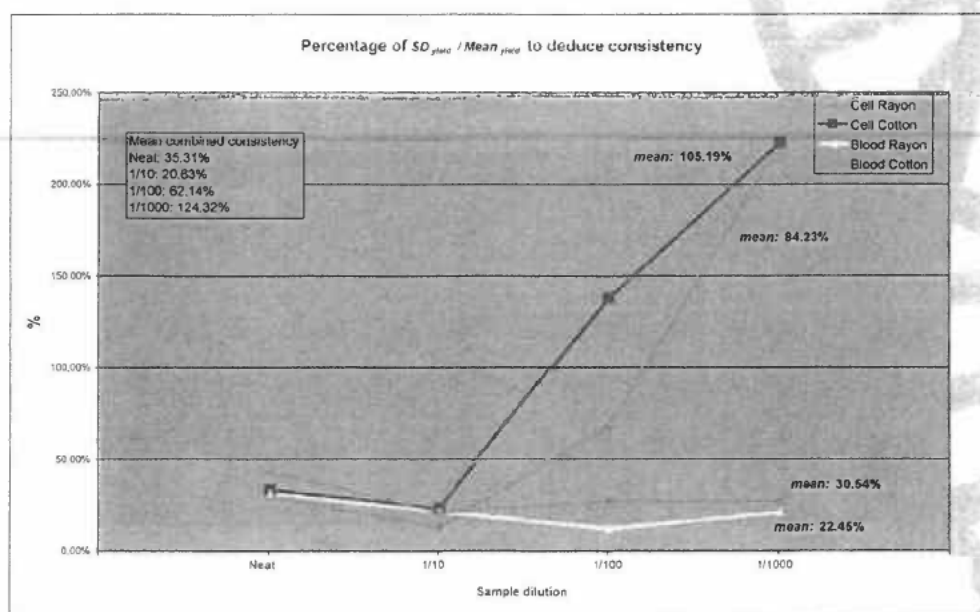


Figure 4. Reproducibility between replicates for cell and blood samples diluted down to 1/1000.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

6.3 Inhibition

Forensic samples that are commonly submitted for DNA analysis often contain inhibitors. These inhibitors may inhibit or significantly reduce the efficiency of a DNA extraction system, either by interfering with cell lysis or interfering by nucleic acid degradation or capture, therefore manifesting as extraction inhibitors (Butler, 2005). Inhibitors can also co-extract with the DNA and inhibit downstream PCR amplification processes, therefore acting as PCR inhibitors (Butler, 2005). For example, inhibitors such as hemoglobin and indigo dye likely bind in the active site of the *Taq* DNA polymerase and prevent its proper functioning during PCR amplification.

For the inhibition study, five substances were chosen for their known ability to inhibit PCR and their likelihood of appearing in routine casework samples:

- Indigo carmine: a component of the blue-dye encountered in denim jeans (Shutler, *et al.*, 1999).
- Tannic acid: a chemical used in the leather tanning process.
- Urea: a component of urine (Mahony *et al.*, 1998).
- Humic acid: a component found in soil and soil products (Tsai and Olson, 1992).
- Motor oil: contains various hydrocarbons and ethanolic compounds that can inhibit PCR.

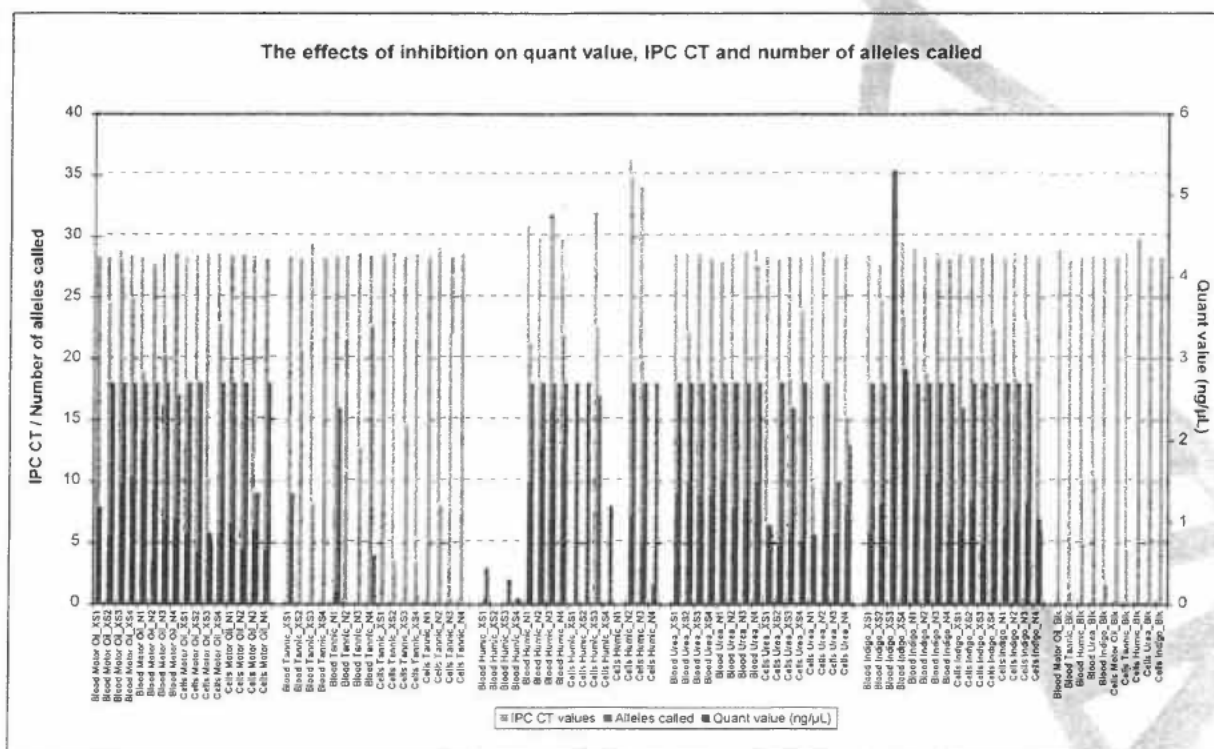


Figure 5. Effects of various inhibitors on quant value, IPC CT and number of resolved alleles.

CaSS | Forensic and Scientific Services

CLINICAL AND STATEWIDE SERVICE

The observed effects of these inhibitors at neat and excess concentrations on the ability to extract, quantify and amplify various DNA samples are graphed in Figure 5. Samples were quantified using the Quantifiler™ Human DNA Quantitation Kit (Applied Biosystems) as this kit includes a built-in inhibition detector. Reaction efficiency and the presence of inhibitors can be assessed based on the performance of the internal positive control (IPC), which is known to be detected in this laboratory at around 28 cycles.

The observations that were made include:

- Samples that were spiked with motor oil, urea and indigo carmine dye did not show inhibition as determined by the IPC, and resulted in quantifiable DNA templates after extraction using DNA IQ™. The average DNA concentration observed for all samples was around 1 ng/μL. The majority of samples yielded full DNA profiles, with the exception of several cell samples that were treated with urea (both at excess and neat concentrations).
- Blood and cell samples that were spiked with tannic acid did not show inhibition in Quantifiler™, as the IPC performed as expected. However, almost no amplifiable template DNA could be quantified and the majority of samples did not produce DNA profiles. This suggests that the original template DNA was degraded by application of tannic acid to the sample. It should be mentioned at this point that the tannic acid used was in the form of a yellow-brown paste substance that was applied directly to the sample swabs. The tannic acid paste, even at the neat concentration, may have been strong enough to severely fragment DNA to result in non-amplifiable templates. It was observed that three blood samples (1 with tannic acid in excess and 2 with tannic acid at neat concentration) yielded partial profiles (between 4-16 reportable alleles), and none of the cell samples produced reportable alleles. This may be caused by: (1) the concentration of viable cells in the buccal cell samples was lower than blood samples; (2) the drying of the blood stain on the substrate may have created a better barrier to protect the blood components from the degradative effects of the tannic acid.
- Blood and cell samples that were treated with humic acid in excess appeared to retain inhibition after extraction using DNA IQ™. However, at neat concentration, the effect of the humic acid inhibitor was overcome and amplifiable DNA template was purified as demonstrated by high DNA concentration yields. Residual inhibition was still present at neat concentration, as evidenced by higher CT values for the IPC (closer to 30), but full profiles were still produced. For some cell samples with humic acid in excess, the Quantifiler™ data suggested full inhibition (undetermined IPC CT and quantitation results), but two samples resulted in full DNA profiles.
- All reagent blanks were undetermined, indicating the absence of contamination in the results.

The results show that the DNA IQ™ system could be used to extract blood or cell samples that were spiked with motor oil, urea and indigo carmine at both excess and neat concentrations. Blood samples that contained humic acid in excess did not yield amplifiable template DNA, but 2 out of 4 cell samples with humic acid in excess appeared to produce full profiles. Samples that were exposed to tannic acid, at both neat and excess concentrations, resulted in non-amplifiable DNA, but the inhibitor was effectively washed out of the extract by DNA IQ™ as evidenced by the amplification of the IPC at the expected CT. Based on these results, we conclude that the DNA IQ™ system effectively removes inhibitors that are present in the original sample, resulting in a DNA extract that is of sufficient quality and is suitable for PCR amplification.

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

6.4 Substrates

The substrate types examined included: swabs (cotton and rayon), tapelifts, fabric (denim, cotton, wool, lycra, nylon, polyester, leather), gum, cigarette butts, and FTA® paper. Cell and blood materials were spotted on to the substrates and extracted using DNA IQ™. The results for the two different sample types are presented in Figures 6 and 7 below.

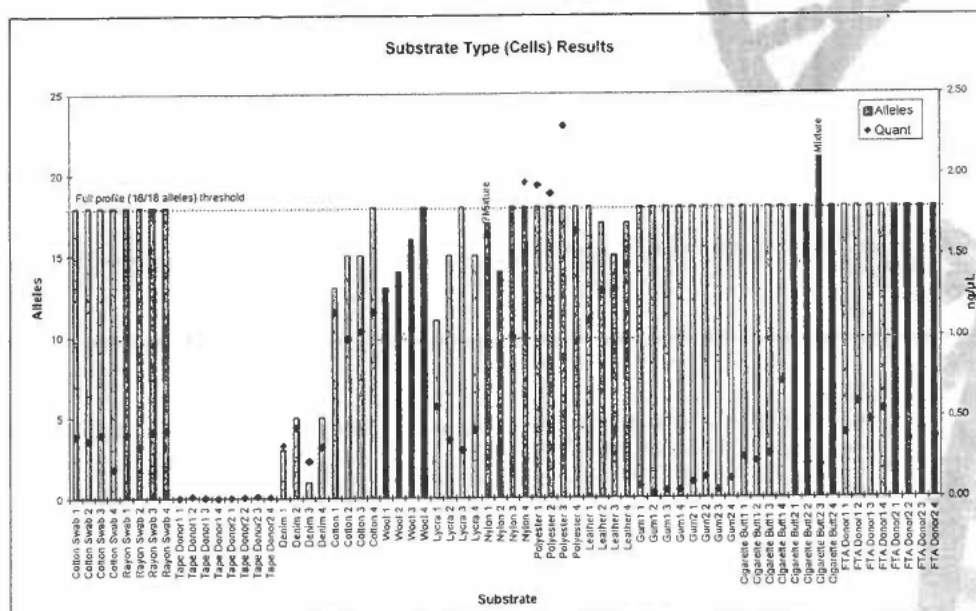


Figure 6. Number of reportable alleles and quantitation results for different substrate types containing cellular material.

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL & STATISTICAL SERVICE

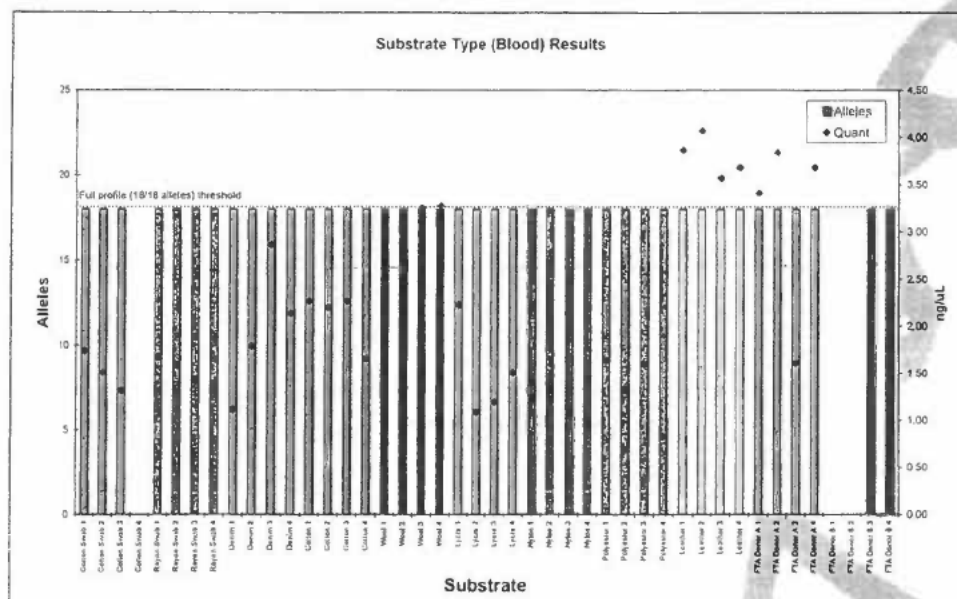


Figure 7. Number of reportable alleles and quantitation results for different substrate types containing blood material.

For cell samples:

- Full DNA profiles (18/18 alleles) were obtained from samples on cotton and rayon swabs, gum, cigarette butts and FTA® paper.
- The quantitation results for most of these samples were less than 0.5ng/μL. For gum samples, the average quantitation result was 0.072ng/μL, and therefore a PCR amplification at maximum volume (20μL) resulted in a total input DNA amount of 1.44ng which is sufficient to result in a full DNA profile.
- Tapelift samples gave an average quantitation result of 0.006ng/μL (just 0.002ng/μL higher than the observed background), and yielded no reportable alleles at all.
- The performance of clothing substrates was variable.
 - Cells on denim yielded quantitation results less than 0.5ng/μL but only partial profiles (maximum 5 reportable alleles), although Quantifiler™ results did not indicate any inhibition of the IPC. The poor performance of these samples may have been a result of sample preparation due to cell clumping.
 - Cells on cotton, wool and nylon resulted in higher quantitation values than lycra, but all substrates generated a similar number of reportable alleles (mean = 14 alleles). Only 25% of samples generated full DNA profiles.
 - Three out of four samples on polyester produced high quantitation results (~2ng/μL) but all samples resulted in a full profile.
 - Cells on leather displayed an average quantitation result of 1.3ng/μL and generated more than 15 reportable alleles.

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

For blood samples:

- All substrate types generated full DNA profiles.
- On average, the DNA quantitation results for all blood samples was greater than those resulted from cell samples. This is as per expected and was observed previously (see Project 9 report), because the concentration of nucleated cells in the blood samples were hypothesised to be higher than the concentration of buccal cell samples.
- Because of processing error, data was not available for the following samples: Cotton Swab 4, FTA Donor B 1 and FTA Donor B 2.

The results above are initial amplification results that do not take into account any reworking options.

We found that samples on tapelift substrates performed the worst; however this was probably due to the sampling method devised for this experiment, which did not adequately sample a sufficient number of cells.

6.5 Mixture studies

A mixture study was performed as part of the validation, however the results are not presented in this document because the mixture ratio was found to be inaccurate because cell counts were not performed on the saliva samples. Therefore, little information could be deduced from these results.

6.6 Substrate size

Blood on cotton swabs produced full DNA profiles for all sample sizes, ranging from 0.5 x 0.5cm to 2.0 x 2.0cm (Figure 8). Cells on cotton swabs did not perform as well (Figure 8), possibly due to the nature of the cells and difficulties in obtaining full DNA profiles from cell samples as observed in previous experiments.

Although the same starting amount of sample was used, it was observed that the 0.5 x 0.5cm samples generated higher quantitation results (therefore, also higher yields) compared to the 2.0 x 2.0cm samples (Figure 8). It appears that extraction efficiency decreases as the substrate surface area increases. This may be due to insufficient mixing and distribution of the lysis buffer over a larger substrate surface area, causing insufficient lysis of cellular material. This observation is in line with other reports that the DNA IQ™ system works more efficiently with smaller samples (Promega, 2006). The resulting IPC CT fell within the narrow range of 27.91 – 28.43 (mean = 28.10), indicating that both small and larger samples resulted in DNA extracts of similar quality, but the overall yield was lower for larger substrates (Figure 8 & 9).

GN-03

CaSS | Forensic and Scientific Services

CLINICAL AND STATISTICAL SERVICE

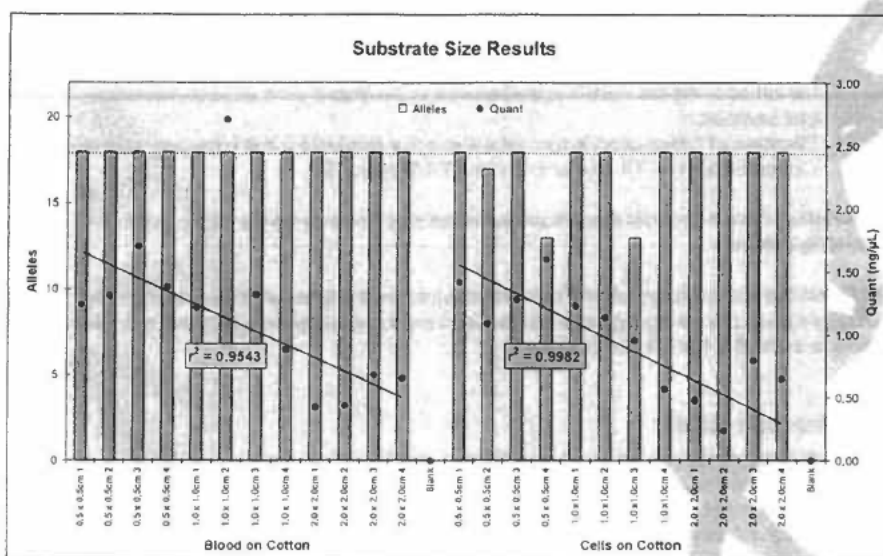


Figure 8 Results for blood and cell samples on cotton substrates of various sizes. All blood samples generated full profiles, but cell samples were more variable. The quantitation results for 0.5 x 0.5cm samples were higher than those for 2.0 x 2.0cm samples (blood $r^2 = 0.9543$; cell $r^2 = 0.9982$; *Note: an outlier was removed from the calculation).

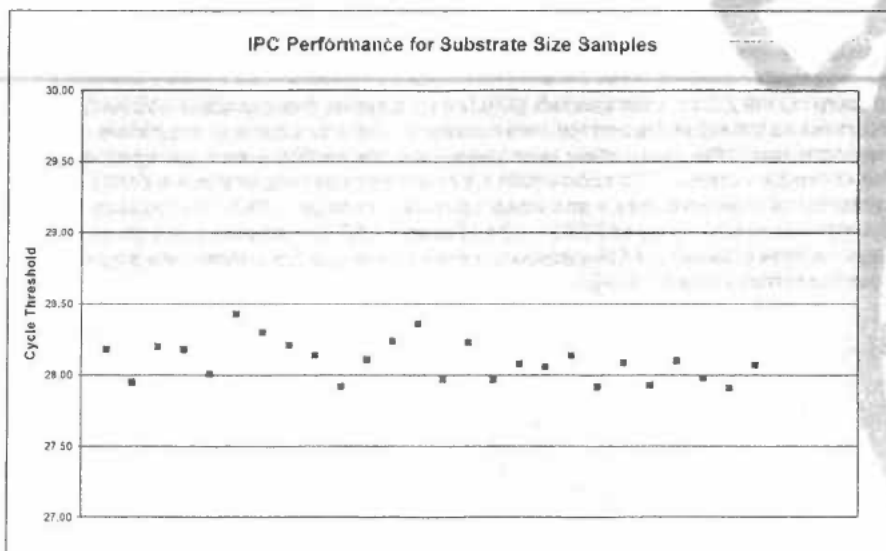


Figure 9. Various sample sizes resulted in similar CT values for the IPC, indicating that IPC performance is not affected by sample size, and that one sample size does not display a level of inhibition that is different to another sample size.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

7. Summary and Recommendations

Based on the findings of this validation report, we recommend:

1. To enable processing of cell and blood samples using the validated manual DNA IQ™ protocol, except for samples on tapelift substrates.
2. To design and verify an automated protocol of the validated DNA IQ™ method for use on the MultiPROBE® II PLUS HT EX platforms, for processing blood and cell samples.

8. Acknowledgements

We wish to thank the Cytology Department at the Royal Brisbane and Women's Hospital for assistance with the cell-counting protocols.

9. References

- Butler JM (2005). *Forensic DNA Typing: Biology, Technology, and Genetics of STR Markers*, 2nd Edition. Elsevier: Burlington, MA, USA.
- Gallagher B, Hlinka V, Iannuzzi C, Lundie G, Muharam I, Nurthen T, Ientile V (2007a). Project 9: Report on the Evaluation of Commercial DNA Extraction Chemistries [Laboratory Report]. DNA Analysis, FSS: Brisbane, QLD, Australia.
- Gallagher B, Hlinka V, Muharam I, Iannuzzi C, Lundie G, Nurthen T, Ientile V (2007b). Mock sample creation for cell and blood samples [Laboratory Report]. DNA Analysis FSS: Brisbane, QLD, Australia.
- Hlinka V, Gallagher B, Iannuzzi C, Lundie G, Muharam I, Nurthen T, Ientile V (2007). Evaluation of the effect of inhibitors as assessed by a silica-based DNA extraction method and real-time PCR [in preparation].
- Huston K (2002). DNA IQ™ System "Frequently Asked Questions". *Profiles in DNA* 5(1):11-12.
- Mahony J, Chong S, Jang D, Luinstra K, Faught M, Dalby D, Sellors J and Chernesky M (1998). Urine specimens from pregnant and nonpregnant women inhibitory to amplification of *Chlamydia trachomatis* nucleic acid by PCR, ligase chain reaction, and transcription-mediated amplification: identification of urinary substances associated with inhibition and removal of inhibitory activity. *Journal of Clinical Microbiology* 36:3122-3126.
- Muharam I, McNevin A, Iannuzzi C, Nurthen T, Ientile V (2007). Project 15: Report on the verification of automated capillary electrophoresis setup using the MultiPROBE® II PLUS HT EX platform [Laboratory Report]. DNA Analysis, FSS: Brisbane, QLD, Australia.
- Mulot C, Stücker I, Clavel J, Beaune P, Lorient M-A (2005). Collection of human genomic DNA from buccal cells for genetic studies: comparison between Cytobrush, mouthwash and treated card. *Journal of Biomedicine and Biotechnology* 2005(3):291-6.
- PerkinElmer (2004). MultiPROBE II Liquid Handling Forensic Workstation Application Guide: Automated DNA IQ™ System for Mixed Casework Sample DNA Isolation [PN 8842157]. PerkinElmer Life and Analytical Sciences: Downers Grove, IL, USA.
- Promega Corporation (2006). DNA IQ™ System – Small Sample Casework Protocol [PN TB296, Rev. 4/06]. Promega Corporation: Madison, WI.
- QIS 15396 R4 (2007). Method for bronchoalveolar lavage (BAL) cell count and differential cell count. [Standard Operating Procedure]. Anatomical Pathology, RBWH: Brisbane, Australia.

GN-03

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

- QIS 19976 R1 (2007). Automated amplification of extracted DNA using the AmpFtSTR® Profiler Plus® or AmpFtSTR® COfiler® kit [Standard Operating Procedure]. DNA Analysis FSS: Coopers Plains, Brisbane, Australia.
- QIS 19977 R1 (2007). Automated quantification of extracted DNA using the Quantifiler™ Human DNA Quantification Kit [Standard Operating Procedure]. DNA Analysis, FSS: Coopers Plains, Brisbane, Australia.
- QIS 19978 R0 (2008). Capillary electrophoresis setup [Standard Operating Procedure]. DNA Analysis, FSS: Coopers Plains, Brisbane, Australia.
- Satia-Abouta, King IB, Abouta JS, Thornquist MD, Bigler J, Patterson RE, Kristal AR, Shattuck AL, Potter JD, White E (2002). Buccal cell DNA yield, quality and collection costs: comparison of methods for large-scale studies. *Cancer, Epidemiology, Biomarkers & Prevention* 11:1130-3.
- Shutler GG, Gagnon P, Verret G, Kalyn H, Korkosh S, Johnston E and Halverson J (1999). Removal of a PCR inhibitor and resolution of DNA STR types in mixed human-canine stains from a five year old case. *Journal of Forensic Sciences* 44(3):623-626.
- Tsai YL and Olson BH (1992). Rapid method for separation of bacterial DNA from humic substances in sediments for polymerase chain reaction. *Applied and Environmental Microbiology* 58(7):2292-2295.

Copyright protects this publication. However, Queensland Health has no objection to this material being reproduced with acknowledgment, except for commercial purposes. Permission to reproduce for commercial purposes should be sought from:

Managing Scientist
DNA Analysis
Forensic and Scientific Services
PO Box 594, Archerfield QLD Australia 4108

Or by telephone (07) 3274 9169

GN-03

*Project 11***Batching Validation Samples ~ Blood****Sensitivity Experiment**

20 Cotton Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_01
 Extracted: CI 12/6/07

20 Rayon Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_02
 Extracted: CI 8/6/07

Inhibition Experiment

8 Indigo Samples
 1 " Blank
 8 Urea Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_03
 Extracted: CI 15/6/07

8 Humic Samples
 1 " Blank
 8 Tannic Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_04
 Extracted: CI 14/6/07

8 Motor Oil Samples
 1 " " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_05
 Extracted: VH 8/6/07

Substrate Experiment

4 Denim Samples
 1 " Blank
 4 Cotton Shirt Samples
 1 " " Blank
 4 Wool Samples
 1 " Blank
 4 Lycra Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_06
 Extracted: CI 13/6/07

4 Nylon Samples
 1 " Blank
 4 Polyester Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_07
 Extracted: CI 7/6/07

4 Rayon Swabs
 1 " Blank
 4 Cotton Swabs
 1 " Blank
 4 FTA Donor 1 Samples
 4 FTA Donor 2 Samples
 1 FTA Blank
 1 Positive Control
 1 Negative Control
VALB20070511_10
 Extracted: GSL 15/6/07

4 Leather Samples
 1 " Blank
 1 Positive Control
 1 Negative Control
VALB20070511_08
 Extracted: CI 5/6/07

GN-03

Mixture Experiment

4 1:1 F:M Samples
4 1:2 F:M Samples
4 1:10 F:M Samples
1 " Blank
1 Positive Control
1 Negative Control
VALB20070605_02
Extracted: GSL 13/6/07

4 1:25 F:M Samples
4 1:50 F:M Samples
4 1:100 F:M Samples
1 " Blank
1 Positive Control
1 Negative Control
VALB20070605_03
Extracted: BG 14/6/07

Size Experiment

12 Cotton Shirt Samples
1 " " Blank
1 Positive Control
1 Negative Control
VALB20070511_11
Extracted: BG 12/6/07

Chemical Validation of a Manual DNA Extraction Method using the DNA IQ™ System

Jenny Lundie, Iman Muharam, Breanna Gallagher, Cecilia Iannuzzi, Vojtech Hlinka, Thomas Nurthen, Vanessa Ientile

Automated, 3MS Implementation Project, DNA Analysis, Forensic and Scientific Services, Queensland Health, 38 Kasloak Rd, Coopers Plains, Brisbane, QLD, Australia 4108

Abstract

We performed an evaluation of various commercial DNA extraction kits, namely DNA IQ™, ChargeSwitch®, QIAamp® DNA Micro, forensiGEM™ and Nucleospin® B Trace in order to compare their overall performance against the current in-house Chelex®-100 protocol. Results of our evaluation identified DNA IQ™ system to be the most suitable kit for extracting oral and blood samples. These samples are routinely analysed in the laboratory. The DNA IQ™ system also outperformed both the current in-house Chelex®-100 protocol and also all the other kits mentioned.

The DNA IQ™ extraction system uses novel paramagnetic resin for DNA isolation to purify DNA without requiring extensive washing to remove the lysis reagent. The DNA IQ™ method was found to generate results that were comparable to or better than the current in-house Chelex®-100 protocols. We validated a manual DNA IQ™ method for extracting DNA from forensic samples and incorporated studies on sensitivity and reproducibility, inhibition, substrate type, substrate size and mixture studies. The validated protocol was based on a modified version of the DNA IQ™ method that is amenable to automation.

The modified protocol includes:
The lysis of sample in Extraction Buffer consisting of TNE buffer (10mM Tris, 100mM NaCl, 1mM EDTA, pH 8.0) Proteinase K (20mg/mL) and SDS (20%) prior to lysis in the DNA IQ™ Lysis Buffer. Reducing the lysis incubation temperature from 70°C to 37°C to allow for heat-sensitive substrates such as nylon and polyester. Increasing the volume of DNA IQ™ Lysis Buffer to allow for the use of Extraction Buffer. Performing a double elution step instead of a single elution step, with a DNA extract volume of 100µL. Incorporating steps to retain supernatant and magnetic beads for storage. This manual DNA IQ™ method is suitable for verification on the automated MultiPROBE® II PLUS HT EX.

Methods

Four donors were chosen for buccal cells and three donors for blood samples. The cells collected on Cytobrush® were resuspended in 2mL of 0.9% saline solution. Whole blood was collected as per standard collection procedures in EDTA tubes by a Phlebotomist. Cytology Department, RBWH performed cell counts for blood and buccal cell samples. Mock samples of five and four replicates were created from the following materials: rayon and cotton swab, gum, cigarette butts, FTA Classic card, tape, fabric materials including denim jeans, cotton shirt, wool, nylon, and polyester. They were placed in sterile 1.5mL tubes. 300µL of neat and diluted sample of blood or buccal cells were applied to all materials. Tape, gum and cigarette butts were not used for the blood validation. A total of five and four replicates of mock samples were created. Samples were dried using a Thermomixer set at 56°C for 2.5 hours in a Class II biohazard cabinet.

The DNA IQ™ Purification System is based on the following:

1. Lysis: cells opened with DTT containing Buffer with or without Proteinase K at 37°C for 45 minutes. 2. Centrifuge: through Spin Basket. 3. Binding: Paramagnetic resin beads selectively bind DNA in presence of optimised reagents. 4. Washing: DNA bound to the beads is held in the magnetic stand while being washed once with Lysis Buffer and then three times with 1x Wash Buffer containing 25% ethanol and 25% isopropanol alcohol (Figure 2). 5. Drying: beads containing DNA are dried to remove remaining inhibitory alcohols. 6. Elution: DNA is eluted from the beads into the elution buffer at 65°C for 5 minutes.

The DNA IQ™ Kit was assessed based on the following experiments:

1. Sensitivity, Reproducibility and Yields using dilutions of cell and blood samples, the dilution were (neat/1/10, 1/100 and 1/1000). 2. Inhibition challenge such as (indigo carmine, motor oil, urea, tannic and humic acid) a total of 300µL of each solution of various inhibitors was applied to the buccal cell and blood swabs prepared previously. 3. Substrate (all fabric materials mentioned). 4. Mixture studies using ratios of (female to male). 5. Substrate size cut into (0.5x0.5cm, 1x1cm and 2x2 cm of cotton shirt). All DNA extracts were quantified using the Quantifiler™ Human DNA Quantitation Kit and were amplified using AmpFISTR® Profiler Plus (Applied Biosystem).

Average yields as observed in the Sensitivity study

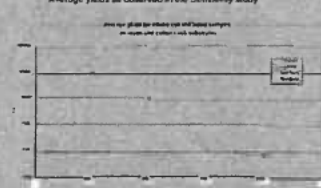


Figure 3: Project 11: Nurthen et al., 2008 DNA Analysis FSS

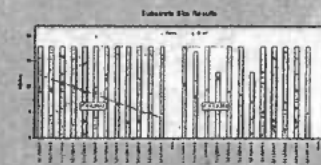


Figure 4: Project 11: Nurthen et al., 2008 DNA Analysis FSS

Results and Discussion

Blood samples produced higher yields compared to cell samples for the sensitivity experiment. As expected neat samples displayed highest yields for five replicates for each (Figure 3). All blood dilutions down to 1/1000 produced quantifiable results and obtained full profiles for cotton swabs and two partial profiles for rayon swabs. For cell samples only dilution down to 1/100 produced reliable quantification, possibly due to inconsistencies in cell suspension uniformity during dilution. Full profiles could be obtained for cell samples that were diluted down to 1/10, however only partial profiles were obtained from samples diluted to 1/100.

For the inhibition experiment, there was no inhibition observed for sample that were spiked with motor oil, urea and indigo carmine as determined by the Quantifiler IPC. After extraction using DNA IQ™ it resulted in quantifiable DNA templates, the majority of the samples produced full DNA profiles. Samples that were spiked with tannic acid did not produce DNA profiles, this suggest that the template DNA was degraded by the application of tannic acid to the sample. It appears that blood and cell samples treated with humic acid in excess, retained inhibition after extraction using DNA IQ™.

For the substrate experiments, full profiles were obtained from cell samples on cotton and rayon swab, gum, cigarette butts and FTA® paper. For clothing materials only partial profiles were obtained. As for tape, it yielded no reportable alleles at all. Less than 0.5ng/µL were obtained for quantification result for most of these samples. For blood samples however, all substrate types generated full profiles. The quantification results produced higher yields in blood compared to cell samples as observed previously (Gallagher et al. 2007).

Results for mixture studies are not presented since cell counts were not performed on buccal samples and the mixture ratio was found to be inaccurate. Consequently not enough information could be assumed from these result.

For all samples in substrate size experiments, blood samples produced full DNA profiles for all sample sizes. However cell samples did not perform well (Figure 4), possibly due to inconsistencies in cell suspension as observed in previous experiments. It was also observed that smaller sizes generated higher quant values compared to bigger sizes. It appears that as the surface area increases, extraction efficiency decreases due to the inadequate distribution of lysis buffer causing insufficient lysis of cellular materials. This observation is in line with other reports that DNA IQ™ system works efficiently with smaller samples (Promega, 2006).

Conclusions

1. Based on overall results of the DNA IQ™ system validation, we concluded that the DNA IQ™ system is suitable for processing cell and blood samples for DNA Analysis, FSS.
2. The DNA IQ™ system can be verify on the MultiPROBE® II PLUS HT EX platforms for automated DNA extraction of various DNA Analysis FSS substrate types.

References

1. Butler JM (2005). Forensic DNA Typing: Biology, Technology, and Genetics of STR Markers, 2nd Edition Elsevier, Burlington, MA, USA. 2. Gallagher B, Hlinka V, Iannuzzi C, Lundie G, Muharam I, Nurthen T, Ientile V (2007a) Project 9 Report on the Evaluation of Commercial DNA Extraction Chemistries (Laboratory Report). DNA Analysis, FSS (Brisbane, Australia). 3. Hlinka V, Gallagher B, Ientile C, Lundie G, Nurthen T, Ientile V (2007b). Evaluation of the effect of inhibitors on automated DNA extraction method and real-time PCR (in preparation). 4. Promega Corporation (2006). DNA IQ™ System, Small Sample Extractor Protocol (PMT3386, Rev 4/06). Promega Corporation/Medison, WI. 5. Nurthen T, Hlinka V, Muharam I, Gallagher B, Lundie G, Iannuzzi C, Ientile V (2008) Project 11: Report on the Validation of a Manual Method for Extracting DNA using the DNA IQ™ System. Automated, 3MS Implementation Project Team, DNA Analysis FSS (Brisbane, Australia). 6. Q15 1536 RI (2007). Method for bronchoalveolar lavage (BAL) cell count and differential count Standard Operating Procedure. Anatomical Pathology, RBWH/Brisbane, Australia.

Acknowledgements

I wish to thank the following for their assistance and support

1. Australian and New Zealand Forensic Science Society, QLD Branch, Australia.
2. Promega Corporation/Medison, WI, USA.
3. Queensland Health, Queensland Government, Australia.
4. DNA Analysis, FSS, (Analytical Section, Automation and L&B4 Implementation Project team) QLD, Australia.

CaSS Forensic and Scientific Services

A CRIMINAL JUSTICE SERVICE

This poster was presented at the 10th International Symposium on the Forensic Sciences (Melbourne, VIC, Oct 6-8, 2008)



Queensland Government
Queensland Health

© The State of Queensland, Queensland Health 2008

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Project 13. Report on the Verification of an Automated DNA IQ™ Protocol using the MultiPROBE® II PLUS HT EX with Gripper™ Integration Platform

Nurthen, T., Hlinka, V., Muharam, I., Gallagher, B., Lundie, G., Iannuzzi, C., Ientile, V.
Automation/LIMS Implementation Project, DNA Analysis FSS (August 2008)

1. Abstract

A manual method for extracting DNA from forensic samples using the DNA IQ™ system (Promega Corp., Madison, WI, USA) was validated for routine use in DNA Analysis (FSS). We have verified an automated DNA IQ™ protocol in 96-well format for use on the MultiPROBE® II PLUS HT EX Forensic Workstation platforms (PerkinElmer, Downers Grove, IL, USA). Data indicate that results from the automated procedure are comparable to those from the manual procedure. Contamination checks were performed using samples prepared in checkerboard and zebra-stripe format, and results were as expected. We recommend the use of the MultiPROBE® II PLUS HT EX platforms to perform automated DNA extraction using the DNA IQ™ system.

2. Introduction

The MultiPROBE® II PLUS HT EX FORENSIC WORKSTATION platforms (PerkinElmer, Downers Grove, IL, USA) are equipped to perform automated DNA extractions, as they include a DPC shaker and individual heat controllers to enable on-board lysis and incubation steps. Currently in DNA Analysis, the MultiPROBE® platforms allow walk-away operation of PCR setup protocols for DNA quantitation and amplification.

The DNA IQ™ protocol has been verified or validated by various laboratories for use on the MultiPROBE® II PLUS platform. The laboratories that perform an automated DNA IQ™ protocol include PathWest (Western Australia), Forensic Science South Australia (South Australia) and Centre of Forensic Sciences in Toronto (Ontario). The MultiPROBE® II PLUS instrument comes pre-loaded with an automated DNA IQ™ protocol. Unlike the other laboratories, however, we did not validate the included protocol, but instead validated a manual DNA IQ™ protocol which was based on the CFS automated protocol (PerkinElmer, 2004), followed by verification of an automated protocol based on the validated manual method.

The verified automated DNA IQ™ protocol is identical to the validated manual protocol used in-house; there are no differences in reagents or volumes. The adopted DNA IQ™ protocol differs slightly, however, from the manufacturer's protocol, as it includes a lysis step using Extraction Buffer (10mM Tris, 1mM EDTA, 100mM NaCl, 20% w/v SDS) in the presence of Proteinase K, before incubating in the DNA IQ™ Lysis Buffer. Furthermore, the lysis incubation conditions were lowered from 70°C to 37°C in order to accommodate extraction of DNA from heat labile materials such as nylon and polyester. In addition, the automated protocol utilises the SlicPrep™ 96 Device (Promega Corp., Madison, WI, USA) for simultaneous processing of samples in a 96-well format.

CaSS | Forensic and Scientific Services

A CLINICAL AND SCIENTIFIC SERVICE

3. Aim

To verify an automated DNA IQ™ protocol for use on the MultiPROBE® II PLUS HT EX platforms to allow extraction of DNA from various sample types.

4. Equipment and Materials

- MultiPROBE® II PLUS HT EX with Gripper™ Integration Platform (PerkinElmer, Downers Grove, IL, USA)
- Gravimetric Performance Evaluation Option with Mettler SAG285/L balance (Mettler-Toledo, Greifensee, Switzerland)
- DNA IQ™ System (Promega Corp., Madison, WI, USA)
- Extraction Buffer (10mM Tris, 1mM EDTA, 100mM NaCl, 20% SDS)
- SlicPrep™ 96 Device (Promega Corp., Madison, WI, USA)
- Nunc™ Bank-It tubes (Nunc A/S, Roskilde, Denmark)
- 175µL non-conductive sterile filter RoboRack tips (PerkinElmer, Downers Grove, IL, USA)
- 1000µL Conductive sterile filter Robotix tips (Molecular BioProducts, San Diego, CA, USA)
- ABI Prism® 7000 SDS (Applied Biosystems, Foster City, CA, USA)
- Quantifiler™ Human DNA Quantification kits (Applied Biosystems, Foster City, CA, USA)
- AmpFtSTR® Profiler Plus Amplification kits (Applied Biosystems, Foster City, CA, USA)
- GeneAmp® 9700 thermalcyclers (Applied Biosystems, Foster City, CA, USA)
- ABI Prism® 96-well optical reaction plates (Applied Biosystems, Foster City, CA, USA)
- ABI Prism® 3100 Genetic Analyzer (Applied Biosystems, Foster City, CA, USA)
- GeneScan™ 500 ROX™ Size Standard (Applied Biosystems, Foster City, CA, USA)
- Hi-Di™ Formamide (Applied Biosystems, Foster City, CA, USA)
- 3100 POP-4™ Polymer (Applied Biosystems, Foster City, CA, USA)
- Cytobrush® Plus Cell Collector (Cooper Surgical, Inc., Trumbull, CT, USA)
- 0.9% saline solution (Baxter Healthcare, Old Toongabbie, NSW, Australia)
- Stem digital tilting head thermometer
- For mock samples:
 - FTA™ Classic Card (Whatman Inc., Florham Park, NJ, USA)
 - Sterile cotton swabs (Medical Wire & Equipment, Corsham, Wiltshire, England)
 - Sterile rayon swabs (Copan Italia SPA, Brescia, Italy)

5. Methods

5.1 Gravimetric Evaluation of Pipetting Accuracy and Precision

Gravimetric analysis was performed by placing the SAG285/L balance on the platform deck and instructing the MP II to repeatedly pipette certain volumes of system liquid onto the balance pan. Readings were taken automatically by the software and compiled into a results table, which was then used to automatically generate an Excel-based results chart containing mean, %CV and %inaccuracy values. The mean values obtained were used to calculate R^2 , slope and Y-intercept (offset) values to calibrate the system's pipetting.

Pipetting performance was assessed for various volumes using three different tips in order to calculate appropriate R^2 , slope and Y-intercept (offset) values which were then added to the performance file. Values were calculated for both Blowout (single-liquid transfer) and Waste (multidispense) modes for the 1000µL conductive tips, and Blowout mode only for the 175µL non-conductive tips and fixed tips.

For the addition of resin, a specialised performance file was created based on the performance file for 175µL tips in blowout mode, except the "Blowout Volume" column values were set to 0 to allow pipetting performance that is similar to waste mode. Retesting was performed to confirm accurate and precise pipetting with these settings.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Figure { SEQ Figure 1* ARABIC }. The Balance Test Information Window as present within the Balance Test DT program. All pipetting parameters are entered here and are subsequently transferred to the result output file.

All gravimetric testing was performed using the Balance Test DT test program within WinPrep®. Parameter values that needed to be entered into the Balance Test Information Window (Figure 1) included those as outlined in Table 1.

Table { SEQ Table 1* ARABIC }. Input values that are required for the various Balance Test Information parameters.

Parameter(s)	Value
Volume 1 and Volume 2	For 175µL tips: 175, 100, 50, 15µL For 1000µL tips: 1000, 700, 400, 100µL For fixed tips: 1000, 700, 400, 100µL
Number of Replicates	10
System Liquid	Degassed Nanopure Water
Sample Type	Nanopure Water
Technician	Initials of the operator performing the test
Sample Density (g/ml)	The density of water at environmental temperature*
Tip Type	Other
Disposable Tip Lot #	The lot number of the particular tips in use
Performance File	The appropriate Performance File for the tip (175µL, 1000µL or fixed tips) and pipetting mode (Blowout or Waste) in use
Enable Tips (checkboxes)	Select the actual tips (1 to 8) to be tested
Comments	Free text box to add additional information (eg. Tip type, mode, current environmental room temperature, etc).

* Water density values were obtained from http://www.simetric.co.uk/si_water.htm

Pipetting accuracy and precision were examined at four different volumes for each tip size: 175, 100, 50, 15µL for 175µL tips and 1000, 700, 400, 100µL for the 1000µL and fixed tips.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

In order to calculate unbiased values for each set of volumes, the slope and offset values in the relevant Performance File were changed to the default 1 and 0 respectively prior to testing. The mean volumes that were pipetted by each tip (10 replicates per tip) at the four designated volumes were used to generate a standard curve. The slope and offset calculated from this curve was used to calibrate the relevant Performance File. The final Performance File settings were then tested at the highest and lowest volumes (as per Table 1) to confirm accurate and precise pipetting.

5.2 Blood Collection

Blood samples were collected from 2 staff donors (DJC/VKI) by a phlebotomist as per normal in three 4mL EDTA vials. Blood samples were stored at 4°C.

5.3 Cell Collection

Buccal cells were collected using a modified Cytobrush® protocol (Mulot *et al.*, 2005; Satia-Abouta *et al.*, 2002). The donor was instructed to brush the inside of one cheek for one minute using a Cytobrush®. Then, with another Cytobrush®, the other cheek was also sampled. Once each cheek was swabbed, the cells on the brush were suspended in 2mL of 0.9% saline solution. Buccal cell samples were stored at 4°C.

5.4 FTA cell Collection

Cells were collected from two staff donors (VKI/CJA) by using a "lolly-pop" swab to sample the inside of the donor's cheek for 15 seconds before pressing the swab onto the FTA™ paper to transfer the DNA. FTA™ cards were stored at room temperature.

5.5 Heater tile temperature verification

Heat tiles supplied with the MultiPROBE® II PLUS HT EX platforms were modified to accept the SlicPrep™ 96 Device. For testing, 1mL of nanopure water (at room temperature) was added to each well. The plate was then placed on a heater tile (controlled by the MP II heater controller) and allowed to reach temperature. The temperatures tested were 37°C and 65°C. Temperature readings for specific outer and inner wells (i.e. A1, A6, A12, D1, D6, D12, H1, H6, H12) were taken at regular intervals up to and including 45 minutes, using calibrated stem digital tilted head thermometer probes. The data were collated and means calculated to determine the distribution of heat over the tile.

5.6 Verification of automated DNA IQ™ Protocol

The automated DNA IQ™ protocol, based on the validated manual method (refer to Project 11), was programmed in WinPrep™ software. The final, optimised protocol was named "DNA IQ Extraction_Ver1.1.mpt". A screenshot of the Test Outline window for this protocol is depicted below in Figure 2. The deck layout is illustrated in Figure 3.

The automated DNA IQ™ protocol was designed to mimic the validated manual method, with minor modifications. Briefly, the changes include:

- Increasing the volume of Extraction Buffer to 500µL;
- A SlicPrep™ 96 Device (Promega Corp., Madison, WI, USA) was used for sample lysis;
- Incubation steps and any shaking steps were performed on the integrated DPC shaker;

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

- CRS toroid magnet (P/N 5083175) was used for isolating the DNA IQ™ resin.
- Instead of a single elution of 100µL, a double elution method (2 x 50µL) is used.

Reagents used in the automated protocol were as per the manual method.

Test Outline

- Initial User Query (x 1)
- BarcodeSetup (x 1)
- ReadBarcode (x 1)
- UserMessage - Hardware setup (x 1)
- Initial Flush/Wash_1 (x 1)
- OpenComm to Shaker (x 1)
- Set Heater Temperature at 37°C (x 1)
- Set Heater Temperature at 65°C (x 1)
- Add 500µl Extraction Buffer to SlicBask (x File: Records)
- Wait for 37 Temperature (x 1)
- Seal plate (x 1)
- ShakerOn_1 (x 1)
- Inubate 45min on heater/shaker_1 (x 1)
- StopShaker_1 (x 1)
- Centrifuge (x 1)
- Place SlicPrep D16 (x 1)
- Flush/Wash_1 (x 1)
- Add Resin 50µl (x File: Records)
- Flush/Wash_3 (x 1)
- Add DNA IQ Lysis Buffer (957 µl) to SlicPrep at D16 (x File: Records)
- Flush/Wash_1 (x 1)
- Move Plate_1 (x 1)
- ShakerOn_2 (x 1)
- Time 5 min_1 (x 1)
- StopShaker_2 (x 1)
- Move SlicPrep to PKI Magnet (x 1)
- Time 1 min - Wait to Bind Resin_1 (x 1)
- Remove 1600µl to AxSuper (x File: Records)
- Flush/Wash_3 (x 1)
- Move SlicPrep to shaker (x 1)
- Dispense Lysis Buffer (125 µl) (x File: Records)
- Flush/Wash_4 (x 1)
- ShakerOn_3 (x 1)
- Timer_1 (x 1)
- StopShaker_3 (x 1)
- Flush/Wash_1 (x 1)
- Move SlicPres to PKI Magnet (x 1)
- Time 1 minute (x 1)
- Remove Lysis Buffer (125 µl) to STORE (x File: Records)
- Move SlicPrep from PKI Magnet to Shaker 1 (x 1)
- Add wash buffer 1 (x File: Records)
- Flush/Wash_1 (x 1)
- ShakerOnWash1 (x 1)
- Shake 1 minute.Wash1 (x 1)
- StopShakerWash1 (x 1)
- Flush/WashWash1 (x 1)
- Move Plate SlicPrep to PKIMagnetWash1 (x 1)
- Bind 1 minute_Wash1 (x 1)
- Remove wash buffer 1 (x File: Records)
- Move SlicPrep from PKI Magnet to Shaker 2 (x 1)
- Add wash buffer 2 (x File: Records)
- Flush/Wash_2 (x 1)
- ShakerOnWash2 (x 1)
- Shake 1 minute.Wash2 (x 1)
- StopShakerWash2 (x 1)
- Flush/WashWash2 (x 1)
- Move Plate SlicPrep to PKI MagnetWash2 (x 1)
- Bind 1 minute_Wash2 (x 1)
- Remove wash buffer 2 (x File: Records)
- Move SlicPrep from PKI Magnet to Shaker 4 (x 1)
- Add wash buffer 3 (x File: Records)
- Flush/Wash_3 (x 1)
- ShakerOnWash3 (x 1)
- Shake 1 minute.Wash3 (x 1)
- StopShakerWash3 (x 1)
- Flush/WashWash3 (x 1)
- Move Plate SlicPrep to PKI MagnetWash3 (x 1)
- Bind 1 minute_Wash3 (x 1)
- Remove wash buffer 3 (x File: Records)
- Dry 5 minutes (x 1)
- Flush/Wash_4 (x 1)
- Wait for 65 Temperature_1 (x 1)
- Add Elution Buffer (60µl) Elut1 (x File: Records)
- Move SlicPrep from PKI Magnet to Tie2 on Shaker_1 (x 1)
- 3 minutes Timer_1 (x 1)
- ShakerOnElut1 (x 1)
- Shake 3 minute.Elut1 (x 1)
- StopShakerElut1 (x 1)
- Move SlicPrep from Tie2 to PKI Magnet_1 (x 1)
- Push Down SlicPrep Elut1 (x 1)
- Bind 1 minute.Elut1 (x 1)
- Transfer Eluted DNA_Elut1 (x File: Records)
- Flush/Wash_Elut1 (x 1)
- Add Elution Buffer (60µl) Elut2 (x File: Records)
- Move SlicPrep from PKI Magnet to Tie2 on Shaker_2 (x 1)
- 3 minutes Timer_2 (x 1)
- ShakerOnElut2 (x 1)
- Shake 3 minute.Elut2 (x 1)
- StopShakerElut2 (x 1)
- Move SlicPrep from Tie2 to PKI Magnet_2 (x 1)
- Push Down SlicPrep Elut2 (x 1)
- Bind 1 minute.Elut2 (x 1)
- Transfer Eluted DNA_Elut2 (x File: Records)
- Flush/Wash_6 (x 1)
- Close Heater Comm (x 1)
- Close Shaker Comm (x 1)
- Remove Nunc tubes (x 1)
- Amphyl concentrate (x 8)
- Amphyl dilute (x 8)
- Water wash (x 8)
- Flush/Wash_5 (x 2)
- End of Test

CaSS | Forensic and Scientific Services

A CRIMINAL AND STATEWIDE SERVICE

Figure 2. The Test Outline window displaying individual nodes within the DNA IQ Extraction_Ver1.1.mpt program test file.

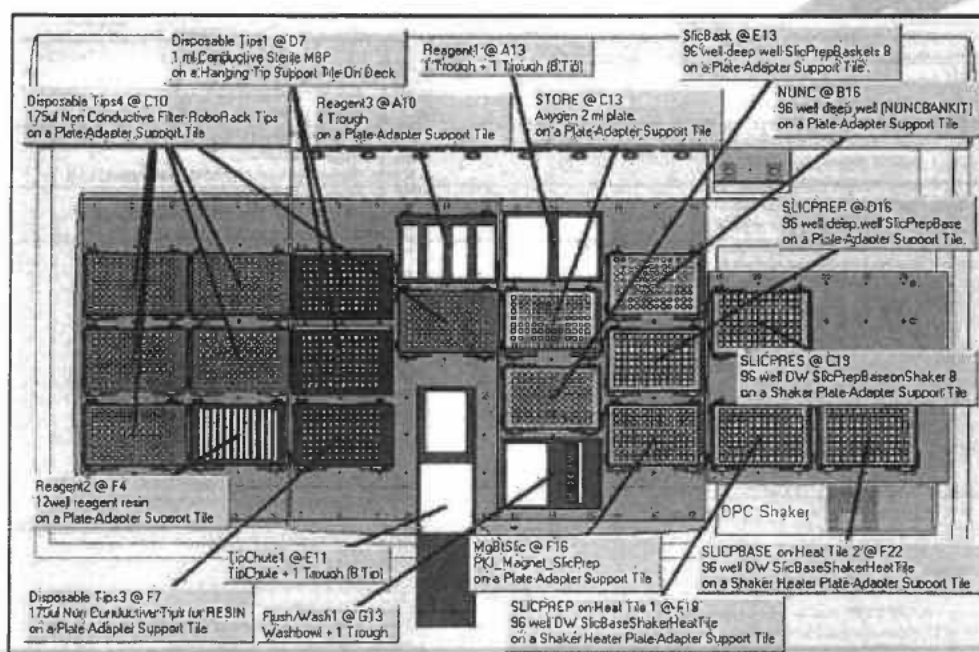


Figure 3. The deck layout for DNA IQ Extraction_Ver1.1.mpt, displaying the required labware on the platform deck.

The automated DNA IQ™ protocol was used to perform the following tests.

5.6.1. Contamination Check via Checkerboard and Zebra-stripe Patterns

Samples consisting of two 3.2mm FTA® discs (containing blood, buccal cells, or blank cards) were arranged in a checkerboard and zebra-stripe pattern (Figure 4) in SlcPrep™ plates using the BSD Duet 600 instrument (BSD Robotics, Brisbane, QLD, Australia) and extracted on the MultiPROBE® II PLUS HT EX platforms using the automated DNA IQ™ protocol. One checkerboard and one zebra-stripe plate was processed on each platform.

GN-05

FSS.0001.0084.1450

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

(a) Checkerboard Pattern

b) Zebra Stripe Pattern

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

Legend:

	Blood FTA®
	Blank FTA®
	Buccal Cell FTA®

Figure 4. Checkerboard and zebra-stripe patterns utilised in the contamination check.

5.6.2. Comparisons with the manual DNA IQ™ method

Comparisons were made between results generated by the automated and manual methods to verify the performance of the automated DNA IQ™ protocol.

Verification samples consisted of different dilutions of blood and cells spotted in 30µL aliquots onto quartered cotton and rayon swabs. Four blood dilutions of neat, 1/10, 1/100 and 1/1000 and four cell dilutions of neat, 1/5.2, 1/52.2 and 1/522 were used to test the sensitivity of both the manual and automated methods. Dilutions were created using 0.9% saline solution for both sample types. Four replicates of each dilution were made up for each substrate and sample type.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

The blood was collected using the same method as in 5.2. Four separate extractions were performed for the manual set based on the combination of sample type and swab type: Blood Rayon, Blood Cotton, Cell Rayon and Cell Cotton. For the automated verification, all sample types were extracted together after being transferred to a SlicPrep™ 96 Device to allow automated processing.

5.6.3. Resin volume

The performance of the automated DNA IQ™ protocol was assessed when either 7µL or 14µL of DNA IQ™ resin was used in the protocol to extract blood samples.

5.6.4. Modifying extraction volumes

The performance of the automated DNA IQ™ protocol was assessed for varying volumes of extraction buffer at 300, 350, 400, 450 and 500µL. In each case, the volume of DNA IQ™ Lysis Buffer was kept at 2x the volume of extraction buffer. Samples extracted were blood swabs, prepared as [REDACTED].

5.6.5. Sensitivity of the automated DNA IQ™ protocol

The sensitivity of the automated DNA IQ™ protocol was assessed using dilutions of whole blood at neat, 1:10, 1:50, 1:100 and 1:1000.

6. Results and Discussion

6.1 Gravimetric Evaluation of Pipetting Accuracy and Precision

Pipetting on both automated platforms was assessed gravimetrically as per laboratory practice. Gravimetric results indicate that pipetting performance for five different pipetting behaviours using 500µL syringes on the instruments is accurate and precise to within the established threshold of $\pm 5\%$ (Table 2). The maximum CV at the maximum volume was 0.78%, whereas the maximum CV at the minimum volume was 1.1%. The CV for pipetting at lower volumes is expected to be slightly higher than the CV at higher volumes using 500µL syringes, because accuracy at small volumes is harder to achieve with larger syringe sizes. Nevertheless, pipetting on the extraction platforms is limited to a minimum of 50µL, which exhibited a CV of 0.36%.

Table 2. Gravimetric evaluation results for various performance files used on either MP II EXTN A or MP II EXTN B.

Performance File	Max. Vol. µL	Min. Vol. µL	Max. Vol. µL Mean	Max. Vol. %CV	Max. Vol. %Inac.	Min. Vol. µL Mean	Min. Vol. %CV	Min. Vol. %Inac.
EXTN A								
Water Blowout 175µL DT_FW_13112007RESIN.prf	50µL	N/A	49.98	0.36	0.0	N/A	N/A	N/A
Water Blowout 175µL DT_FW_QHSS_13112007.prf	175µL	15µL	172.26	0.21	1.6	[REDACTED]	[REDACTED]	[REDACTED]
WaterWaste 1mL_FW_QHSS_12112007.prf	1000µL	100µL	999.11	0.24	0.1	99.22	0.71	0.8
Water Blowout 1mL DT_QHSS_09112007.prf	1000µL	100µL	1001.02	0.27	0.1	100.65	0.63	0.7
Water Blowout Fixed Tips_08112007.prf	1000µL	100µL	995.97	0.31	0.4	99.6	0.71	0.4
EXTN B								
Water Blowout 175µL DT_FW_25102007RESIN.prf	50µL	N/A	50.12	0.36	0.2	N/A	N/A	N/A
Water Blowout 175µL DT_FW_25102007.prf	175µL	15µL	175.58	0.14	0.3	15.23	1.1	1.5
WaterWaste 1mL DT_FW_QHSS_24102007.prf	1000µL	100µL	1002.39	0.78	0.2	99.56	0.89	0.4
Water Blowout 1mL DT_QHSS_23102007.prf	1000µL	100µL	998.2	0.44	0.2	99.44	0.68	0.6

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Water Blowout Fixed Tips_FW 26102007.prf	1000µL	100µL	998.87	0.68	0.1	100.37	0.74	0.4
--	--------	-------	--------	------	-----	--------	------	-----

6.2 Heater tile temperature verification

Two heater tiles on each MP II platform was verified to reach either 37°C or 65°C, the optimum incubation temperatures for sample lysis and DNA elution respectively (using the DNA IQ™ kit). Each tile, upon completion of the verification process, could only be used for a specific temperature, and as such was labelled appropriately to ensure use of the correct tile for specific incubation steps (Table 3).

Table 3. Verified heater tiles for use in the automated DNA IQ™ protocol.

Extraction platform	Tile number	Heater Controller Setting	Average °C reached	Verified temperature	Incubation Step
EXTN A	3 (45W)	50°C	37°C	37°C	Sample Lysis
EXTN A	1 (45W)	85°C		65°C	DNA Elution
EXTN B	1 (45W)	50°C		37°C	Sample Lysis
EXTN B	2 (45W)	85°C	65°C	65°C	DNA Elution

A slight variation in the incubation temperature to achieve sample lysis is acceptable, because Proteinase K exhibits stable activity and broad specificity over a wide range of temperatures between 20-60°C, at which the serine protease still retains greater than 80% of its activity (Sweeney & Walker, 1993).

The efficiency of the elution step is dependent on heating the sample to 65°C in the presence of DNA IQ™ Elution Buffer (Huston, 2002). If the sample is not sufficiently heated, the extraction yield may be lower than expected. Two heater tiles were able to be verified for this crucial incubation step, with both tiles exhibiting minimal variation.

6.3 Contamination Check via Checkerboard and Zebra-stripe Patterns

Table 4 below lists the Extraction Batch ID's of the contamination checks.

Table 4. Extraction Batch ID's for the various contamination check plates that were processed on the MP II platforms using the automated DNA IQ™ protocol.

Type of plate	Extraction batch Id	Extraction Platform	Check passed
Checkerboard 1	VALB20070817_02	Extraction A	Invalidated
Checkerboard 2	VALB20070803_02	Extraction B	Yes
Zebra-Stripe 1	VALB20070803_03	Extraction A	Yes
Zebra-Stripe 2	VALB20070817_03	Extraction B	Yes
Checkerboard/Zebra	VALB20071022_01	Extraction A	Yes

Checkerboard 1

Position E3 (Sample Cells 6) was known to have been contaminated prior to the start of the extraction. The result showed a mixed DNA profile, with contributing alleles originating from the expected wells (Table 5). In addition to this contamination event, eight of the designated blank samples (positions D3, A10, F1, H5, C4, E4, B7 and E6), two of the cell samples (A1 and B10) and two of the blood samples (F4

GN-05

FSS.0001.0084.1453

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

and G7) all exhibited a partial DNA profile that was previously unknown (Table 5). This profile did not match any of the positive control samples present on the batch. The DNA profile was searched against the Staff Database and no matches were found. The source of this contaminating DNA profile could not be identified.

None of the other blank samples yielded any DNA profile. The rest of the cell and blood samples yielded the correct DNA profile. Although there is no evidence of well-to-well contamination, the unknown DNA profile obtained has invalidated this plate. A further checkerboard/Zebra-Stripe combination plate was performed to ensure...

Table 5. The DNA profile of the unknown contaminant that was observed in Checkboard-1.

Sample description	D3	vWA	FGA	Amel	D8	D21	D18	D5	D13	D7
BIK23-E6	14,17	14,17	22,24	X,Y	11,11	29,32,2	14,15	9,11	11,12	11,13
BIK25-B7	14,17	14,17	22,24	X,Y	11,11	29,32,2	14,15	9,11	11,12	
BIK15-E4	14,17	14,17	22,24	X,Y	11,11	29,32,2	14,15	9,11	11,12	11,13
BIK14-C4		14		X	11	32,2		9		
BIK20-H5	14,14	17,17	20,21	X,X	13,16	29,30	14,16	11,13	11,12	11,11
BIK3-F1	14	17		X	13	29,30	14		12	11
BIK10-D3	14,17	14		X,Y	11	29,32,2	14	9,11		11,13
BIK37-A10	14,17	14	22,24	X,Y	11	29	14	9,11		
Cells19-B10	14,17	14,17	20,21,22,24	X,Y	11,13,16	29,30,	14,15,16	11,15	11,12	11,11
Cells13-A1	14,17	14,17	20,21,22,24	X,Y	11,13,16	29,30,32,32,2,33	14,15,16	9,11,13	11,12	11,13
Blood14-G7	NR,17,18	NR,16	20,21	X,Y	NR,13,14	29,30,31,NR	NR,14	NR,12	10,10	10,NR,12
Blood8-F4	NR,17,18	NR,16,17	20,21,NR,24	X,Y	11,13,14	29,30,NR,NR	14,14	9,11,12	10,NR	10,NR,12
Cells 6-E3	14,17,18	16,17	20,21	X,Y	13,14,16	29,30,31	NR,14,16	11,12,13	10,11,12	10,11,12

Checkerboard 2

None of the blank samples yielded DNA profiles; all of the positive cell and positive blood samples yielded the correct DNA profile. Figure 5 illustrates the DNA quantitation results from this plate. DNA was not detected in any of the blank samples.

GN-05

FSS.0001.0084.1454

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

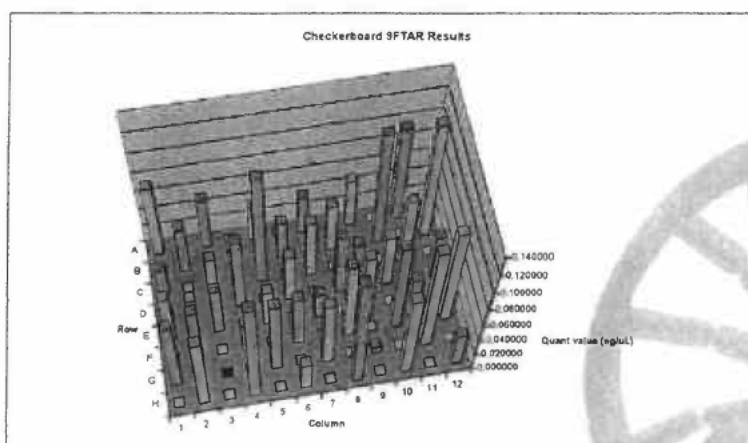


Figure 5. Checkerboard 2 quantitation results, showing the absence of detectable DNA in the blank samples (grey).

Zebra-Stripe 1

None of the blank samples yielded DNA profiles, all of the positive cell and positive blood samples yielded the correct DNA profile. Figure 6 illustrates the absence of detectable DNA in the blank samples.

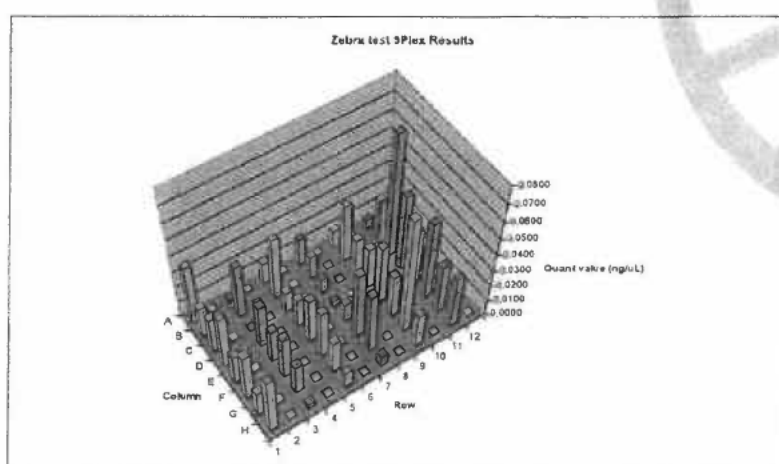


Figure 6. Zebra-Stripe 1 quantitation results, showing the absence of detectable DNA in the blank samples (grey).

Zebra-Stripe 2

None of the blank samples yielded DNA profiles, all of the positive cell and positive blood samples yielded the correct DNA profile. Figure 7 shows the absence of detectable DNA in the blank samples.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

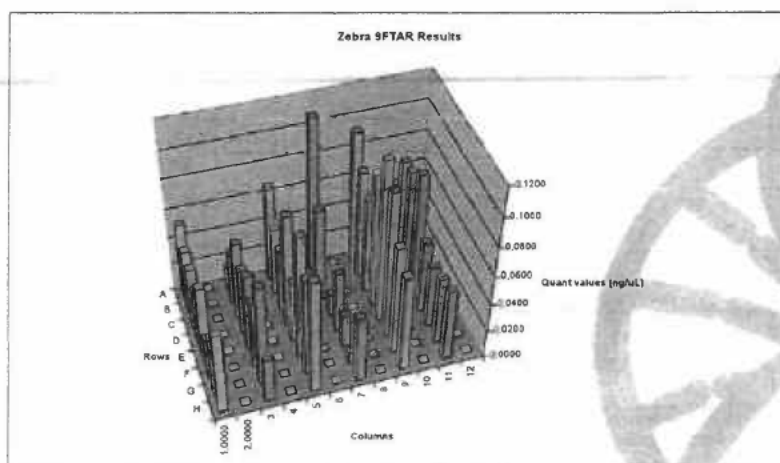


Figure 7. Zebra-Stripe 2 quantitation results, with no DNA detected in the blank samples.

Checkerboard/Zebra

None of the blank samples yielded DNA profiles, all of the positive cell and positive blood samples yielded the correct DNA profile. DNA was undetected in the blank samples (Figure 8).

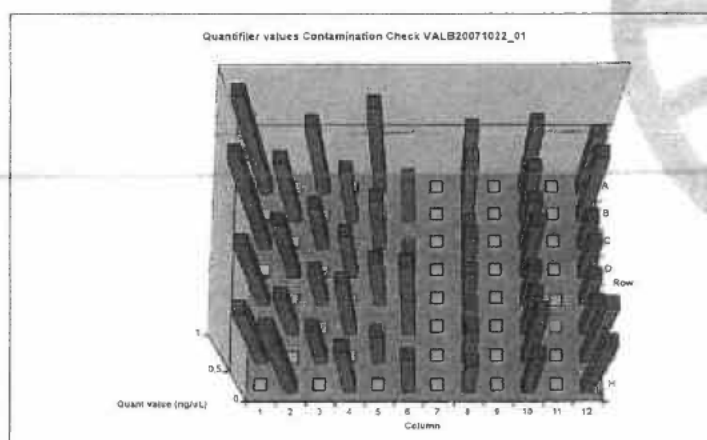


Figure 8. Checkerboard/zebra plate that was extracted on MP II Extraction Platform A because the previous plate was invalidated. DNA was not detected in the blank samples (grey).

6.4 Comparisons with the manual DNA IQ™ method

When dilutions of either blood or cells were applied on to either rayon or cotton swabs, followed by extraction using the DNA IQ™ method, the results of the automated method were always lower in yield compared to the manual method. For blood samples on rayon

CaSS | Forensic and Scientific Services

A CLINICAL AND STATISTICAL SERVICE

swabs, the automated method generated yields that were on average around 8% (SD 8.45%) of the automated method. For blood on cotton swabs, the yield from the automated method was also around 8% (SD 3.62%). The yields for cell samples were higher at around 33% (SD 16.29%) and 25% (10.32%) for cells on rayon and cotton swabs respectively.

The manual method was found to be more sensitive than the automated method. Out of five replicates at the 1/100 and 1/1000 dilutions for blood on rayon swabs that were processed using the manual method, five and three replicates respectively were detected (and none from the automated method) (see Figure 9). The trend is repeated for blood on cotton swabs (Figure 10). For cell samples on either rayon or cotton swabs, the automated method was found to be more sensitive as evidenced by detection of DNA at the 1/522 dilutions (Figure 11 and 12).

Cell clumping may have occurred with the cell dilutions, therefore causing inaccurate dilutions as can be observed in the ratios between each dilution.

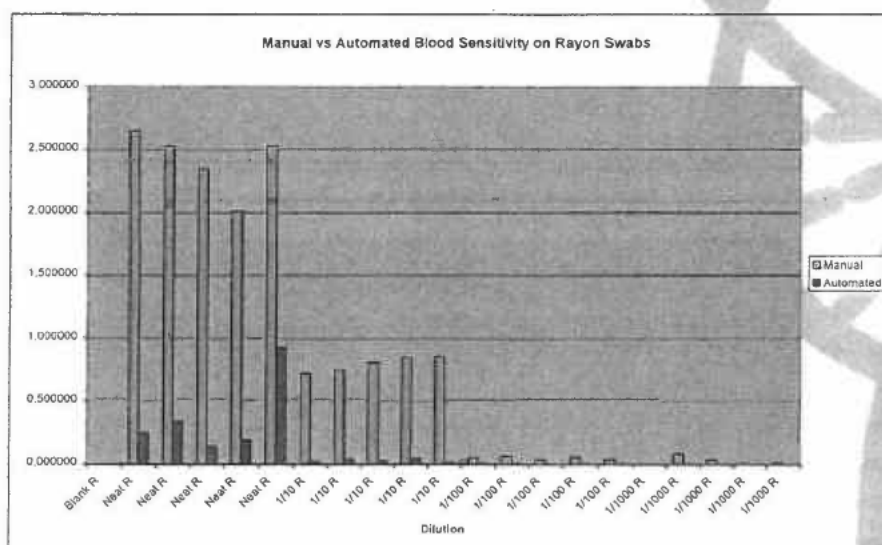


Figure 9. Comparison of sensitivity between the manual and automated DNA IQ™ methods for blood samples on rayon swabs.

GN-05

FSS.0001.0084.1457

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

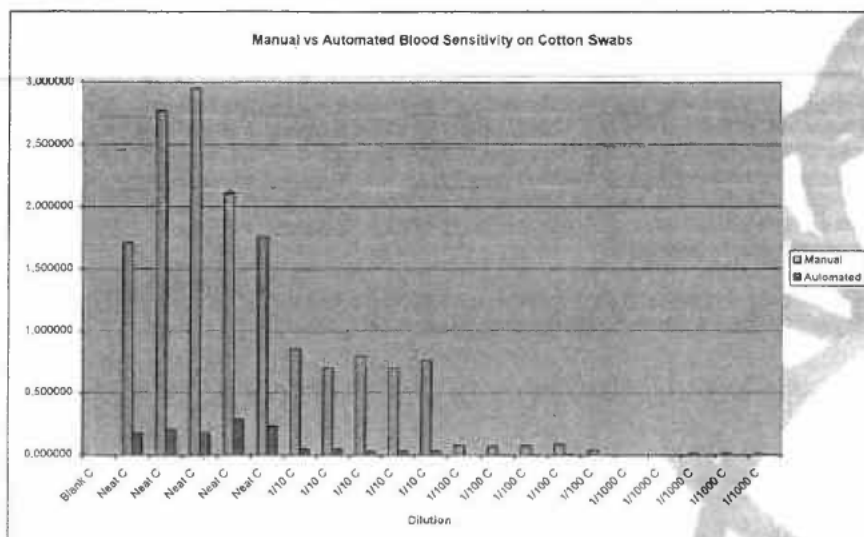


Figure 10. Comparison of sensitivity between the manual and automated DNA IQ™ methods for blood samples on cotton swabs.

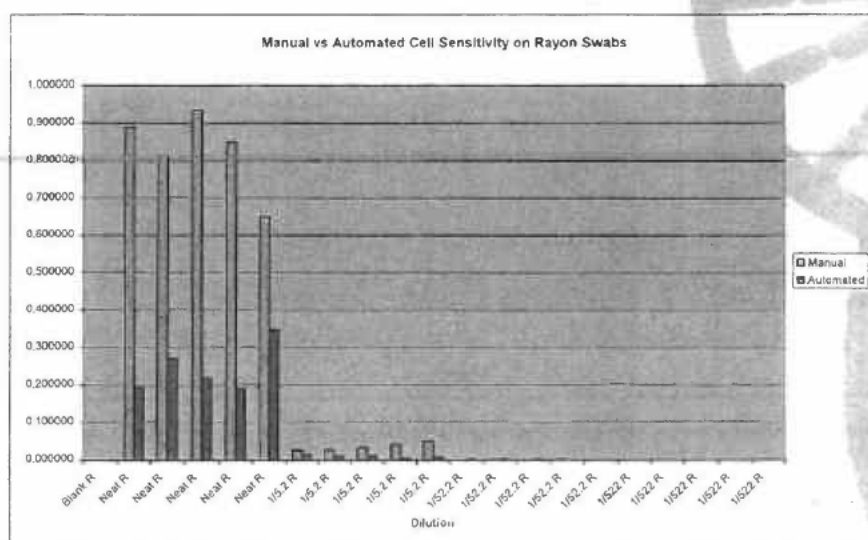


Figure 11. Comparison of sensitivity between the manual and automated DNA IQ™ methods for cells samples on rayon swabs.

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

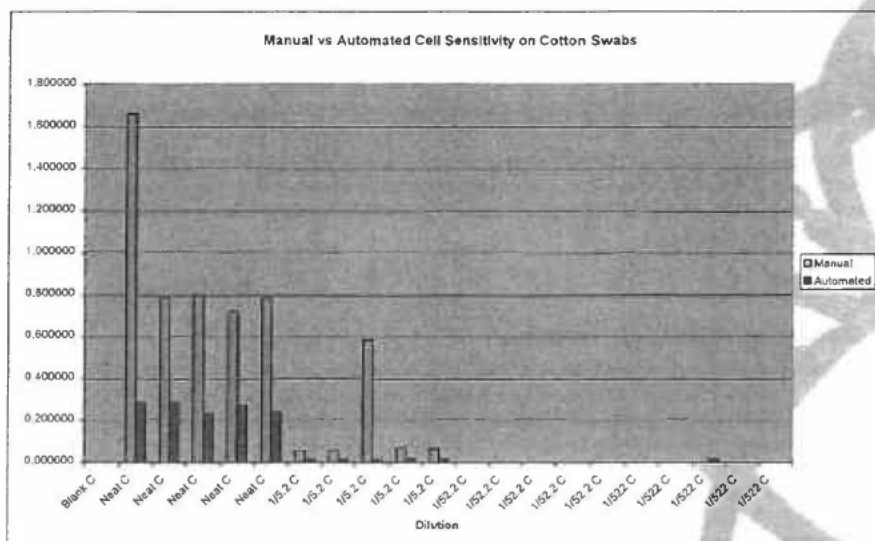


Figure 12. Comparison of sensitivity between the manual and automated DNA IQ™ methods for cell samples on cotton swabs.

6.5 Investigating resin volume

Promega recommends the use of 7µL of DNA IQ™ resin with their protocol. We investigated the performance of the protocol with double the amount of resin (14µL) in order to assess any benefits that may be gained in terms of the resulting yield and quality of the STR profile.

It was observed that doubling the resin resulted in a proportional doubling of the yield. On average, doubling the resin increased the yield by an additional 77.28% ($n=4$). The average yield from an extraction using 7µL of resin was 64.725ng (SD 32.21ng, $n=4$), whereas 14µL resin generated 114.75ng (SD 10.72ng, $n=4$) (Table 6). At the higher resin concentration, the amount of DNA isolated appears to be capped at around 100ng, indicating no change in the ability of the reaction to isolate more DNA due to saturation of resin.

Table 6. Comparison of the effects of doubling the amount of recommended DNA IQ™ resin.

Sample ID	Resin volume	[DNA] ng/µL	Reportable alleles
33383-4216	7µL	0.701	18/18
33383-4225		1.070	18/18
33383-4239		0.319	18/18
33383-4248		0.499	18/18
33383-4252	14µL	1.140	18/18
33383-4261		1.270	18/18
33383-4270		1.010	18/18
33383-4284		1.170	18/18

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

Samples extracted using either amount of resin generated concordant full DNA profiles (18/18 alleles). Samples processed using the 14 μ L method produced peaks that were slightly higher. The difference in peak heights between alleles within the same loci ranged from 59-86%, with a mean of 71%, indicating minimal difference between the two methods.

Doubling the amount of resin did not appear to provide any additional benefits compared to the original recommended protocol. More importantly, full DNA profiles were resolved using either method. Therefore, the costs associated with increasing the amount of resin cannot be justified at this stage.

6.6 Modifying extraction volumes

An investigation into optimising extraction volumes ranging from 300 μ L to 500 μ L was performed in order to ensure that buffer coverage over the samples was sufficient to enable optimal lysis and release of DNA. In addition, the use of an optimum volume of extraction reagents increases efficiency and economy, therefore potentially lowering laboratory costs.

Although the higher extraction volume generated higher yields when processed using the automated DNA IQ™ protocol (Table 7), DNA profile results were comparable across the various extraction volumes tested for eight replicates each (Table 8). Three instances of allelic imbalance were encountered in two samples from the 300 μ L and 450 μ L tests. In all instances, allelic imbalance was greater than 69%.

Table 7. DNA profile results for samples extracted using various volumes of Extraction Buffer, for 8 replicates.

Extraction Buffer Volume (μ L)	Mean [DNA] (ng/ μ L)	SD
300	2.04	0.07
350	2.16	0.09
400	1.69	0.10
450	3.14	0.13
500	3.64	0.17

Table 8. DNA profile results for samples extracted using various volumes of Extraction Buffer, for 8 replicates.

Sample	Extraction Buffer Volume (μ L)	DNA Profile Result
300-1 swab	300	OK
300-2 swab		OK
300-3 swab		OK
300-4 swab		OK
300-5 swab		OK
300-6 swab		OK
300-7 swab		AI D13
300-8 swab		OK

CaSS | Forensic and Scientific Services

A CLINICAL AND STATEWIDE SERVICE

350-1 swab		OK
350-2 swab		OK
350-3 swab		OK
350-4 swab	350	OK
350-5 swab		OK
350-6 swab		OK
350-7 swab		OK
350-8 swab		OK
400-1 swab		OK
400-2 swab		OK
400-3 swab		OK
400-4 swab	400	OK
400-5 swab		OK
400-6 swab		OK
400-7 swab		OK
400-8 swab		OK
450-1 swab		OK
450-2 swab		OK
450-3 swab		OK
450-4 swab	450	OK
450-5 swab		OK
450-6 swab		OK
450-7 swab		AI vWA, D18
450-8 swab		OK
500-1 swab		OK
500-2 swab		OK
500-3 swab		OK
500-4 swab	500	OK
500-5 swab		OK
500-6 swab		OK
500-7 swab		OK
500-8 swab		OK

6.7 Sensitivity of the automated DNA IQ™ protocol

DNA was detected from samples that were diluted down to 1:1000 (Figure 13).

